

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN052813\HN005283.D Vial: 5
Acq On : 28-May-2013, 14:21 Operator: QM
Sample : E2136-03 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: May 28 14:31 2013 Quant Results File: HN052813.RES

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN052813.M
Title :
Last Update : Tue May 28 14:18:38 2013
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.53	508586	0.123 ng/uL

Target Compounds

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.


HN005283.D HN052813.M Tue May 28 14:31:52 2013 RPT1


Quantitation Report

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN052813\HN005283.D Vial: 5
Acq On : 28-May-2013, 14:21 Operator: QM
Sample : E2136-03 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: May 28 14:31 2013 Quant Results File: HN052813.RES

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN052813.M
Title :
Last Update : Tue May 28 14:18:38 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

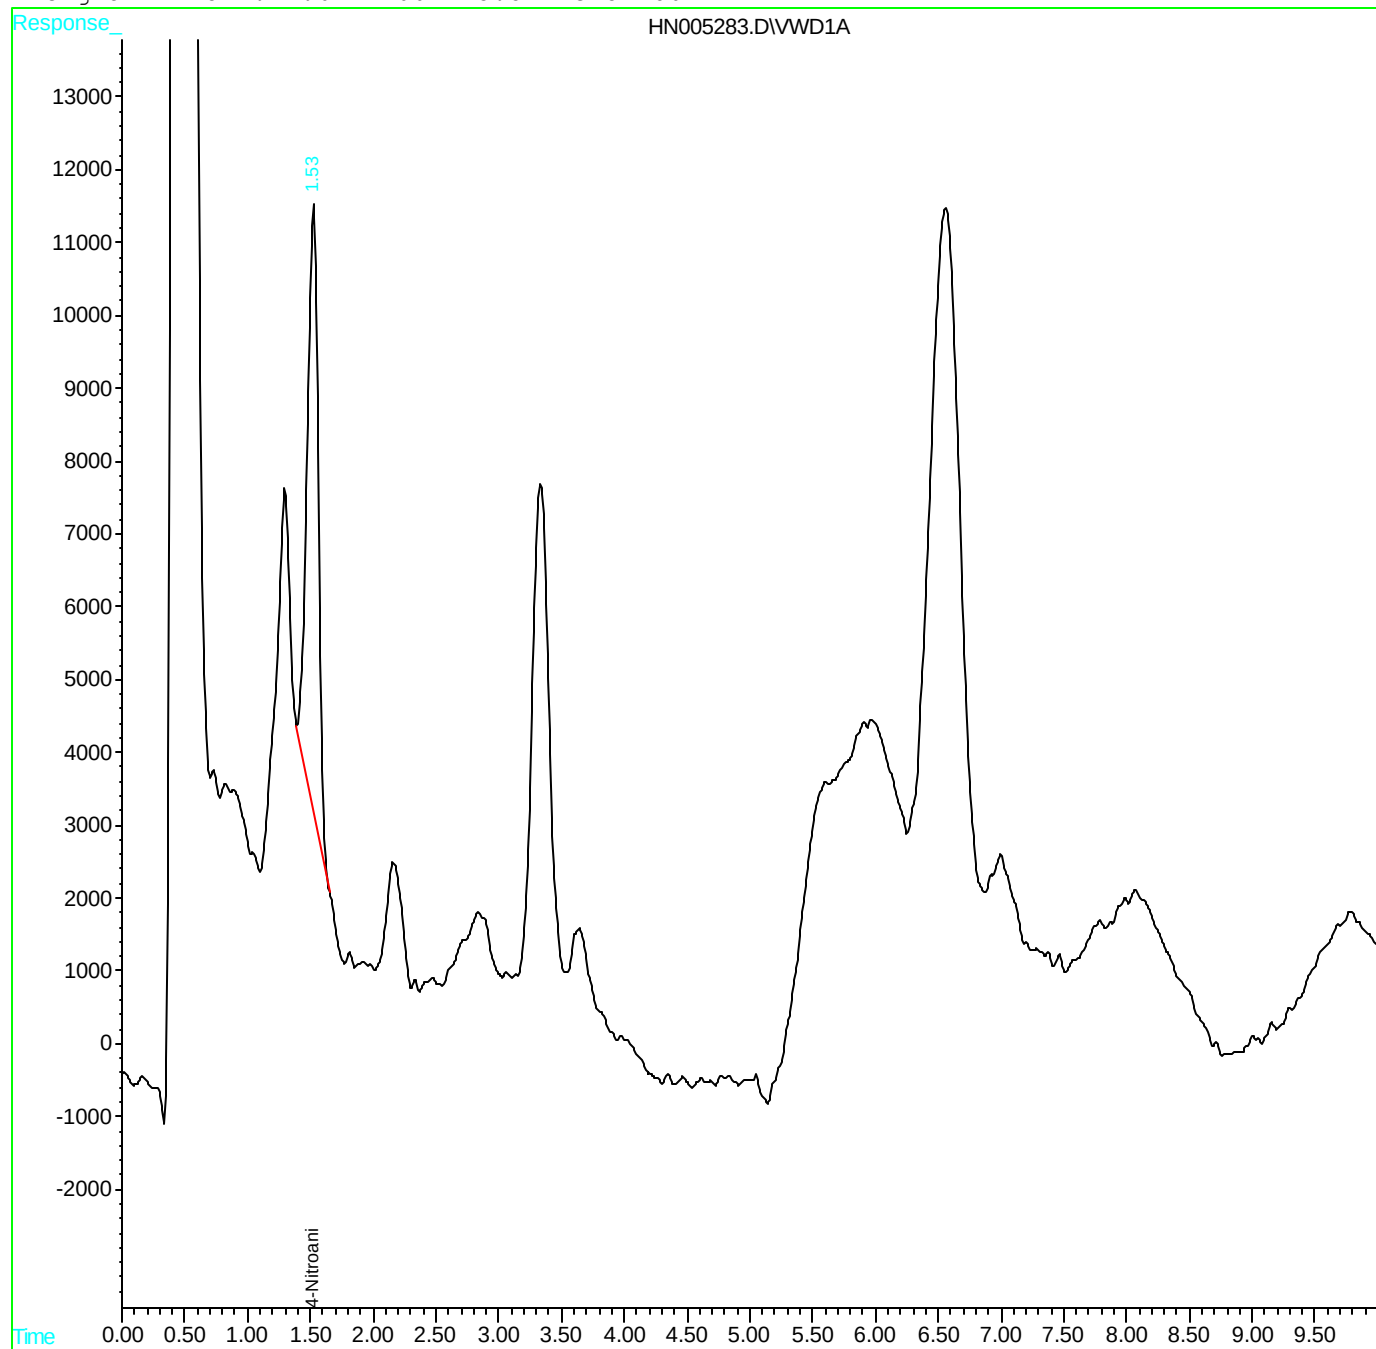

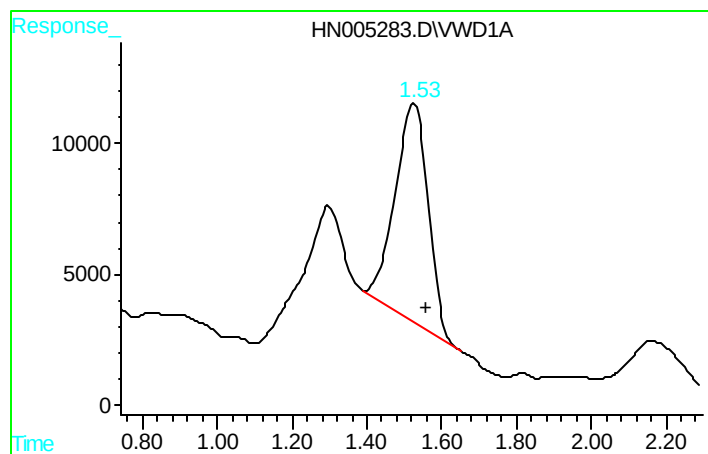

#1 4-Nitroaniline

R.T.: 1.526 min
Delta R.T.: -0.034 min
Response: 508586
Conc: 0.12 ng/uL