

Data File : Z:\HPCHEM1\HPLC\_N\DATA\HN052813\HN005274.D Vial: 3  
Acq On : 28-May-2013, 11:33 Operator: QM  
Sample : HSTDICC010 Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : autoint1.e  
Quant Time: May 28 12:51 2013 Quant Results File: HN052813.RES

Instrument :  
HPLC\_N  
LabSampleId :  
HSTDICC010

Quant Method : Z:\HPCHEM1\HPLC\_N\METHOD\HN052813.M  
Title :  
Last Update : Tue May 28 12:45:46 2013  
Response via : Initial Calibration  
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

| Compound                    | R.T. | Response | Conc Units  |
|-----------------------------|------|----------|-------------|
| -----                       |      |          |             |
| System Monitoring Compounds |      |          |             |
| 1) S 4-Nitroaniline         | 1.56 | 42420994 | 9.716 ng/uL |
| Target Compounds            |      |          |             |
| 2) T Nitroglycerin          | 7.20 | 89621204 | 9.998 ng/uL |

-----  
Analyst Signature:\_\_\_\_\_ Analyst Name:\_\_\_\_\_ Date:\_\_\_\_\_

-----REASONS FOR MANUAL INTEGRATIONS-----

\_\_\_Poor resolution of peaks exhibited on chromatogram.Compound #:\_\_\_\_\_

\_\_\_Peak Integrated by software incorrectly.Compound #:\_\_\_\_\_

\_\_\_OTHER:\_\_\_\_\_Compound #:\_\_\_\_\_

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005274.D HN052813.M

Tue May 28 14:04:56 2013

RPT1


# Quantitation Report


Data File : Z:\HPCHEM1\HPLC\_N\DATA\HN052813\HN005274.D Vial: 3  
Acq On : 28-May-2013, 11:33 Operator: QM  
Sample : HSTDICC010 Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : autoint1.e  
Quant Time: May 28 12:51 2013 Quant Results File: HN052813.RES

Instrument :  
HPLC\_N  
LabSampleId :  
HSTDICC010

Quant Method : Z:\HPCHEM1\HPLC\_N\METHOD\HN052813.M  
Title :  
Last Update : Tue May 28 12:45:46 2013  
Response via : Multiple Level Calibration  
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

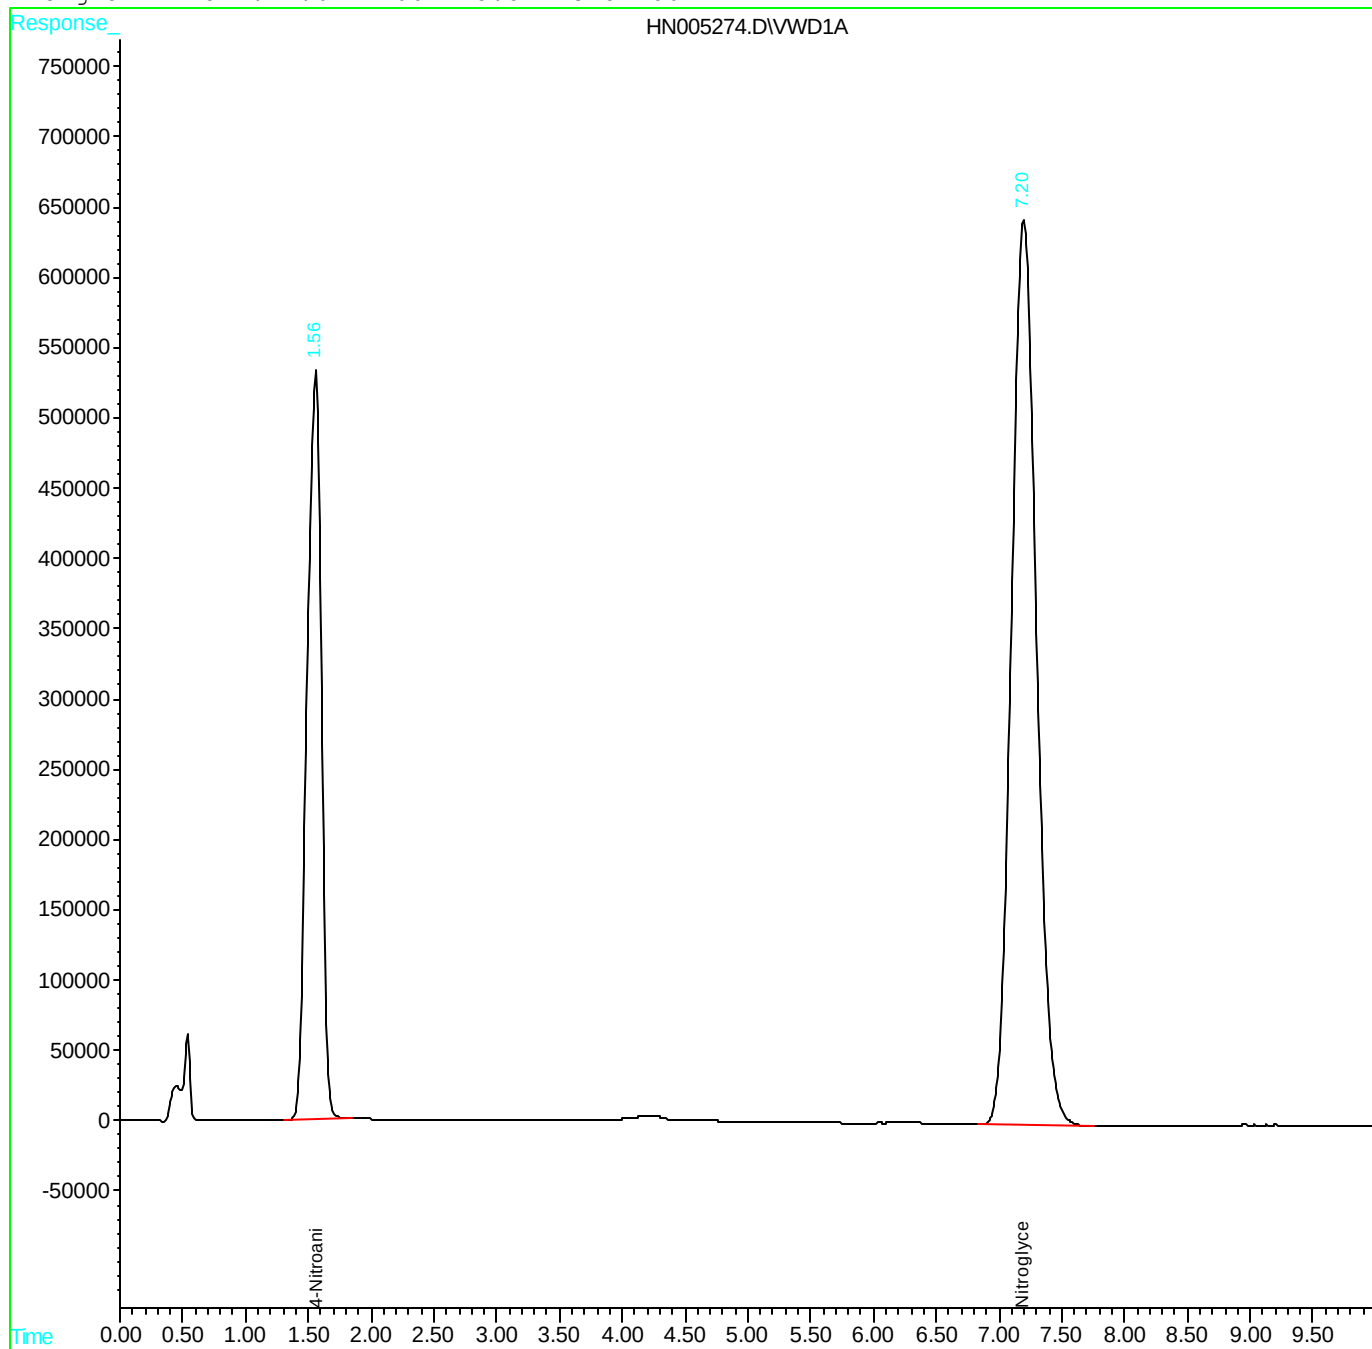


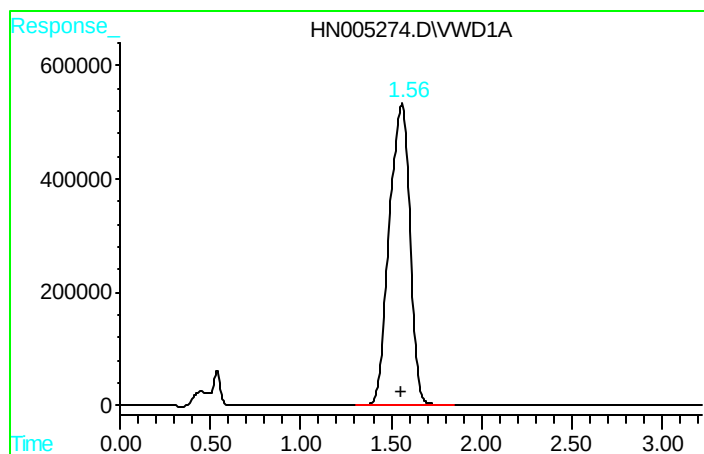

#1 4-Nitroaniline

R.T.: 1.562 min  
 Delta R.T.: 0.012 min  
 Response: 42420994  
 Conc: 9.72 ng/uL

Instrument :  
 HPLC\_N  
 LabSampleId :  
 HSTDIC010

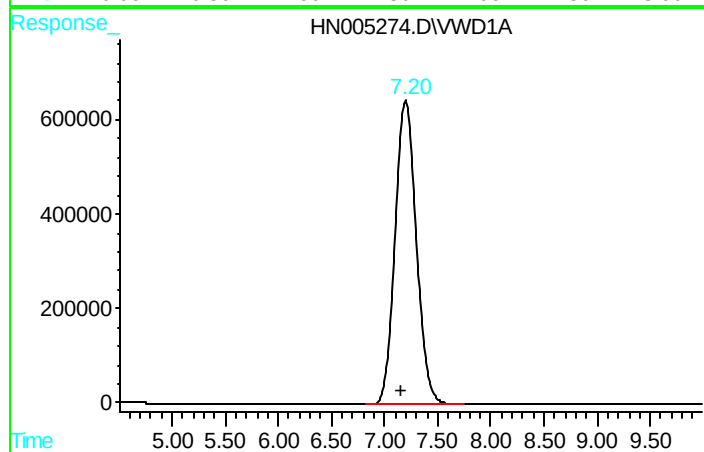

#2 Nitroglycerin

R.T.: 7.198 min  
 Delta R.T.: 0.042 min  
 Response: 89621204  
 Conc: 10.00 ng/uL