

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN052813\HN005276.D Vial: 5
Acq On : 28-May-2013, 11:58 Operator: QM
Sample : HSTDICC001 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: May 28 12:51 2013 Quant Results File: HN052813.RES

Instrument :
HPLC_N
LabSampleId :
HSTDICC001

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN052813.M
Title :
Last Update : Tue May 28 12:45:46 2013
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.55	4094704	0.938 ng/uL
Target Compounds			
2) T Nitroglycerin	7.15	8928553	0.996 ng/uL

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005276.D HN052813.M

Tue May 28 14:07:17 2013

RPT1


Quantitation Report


Data File : Z:\HPCHEM1\HPLC_N\DATA\HN052813\HN005276.D Vial: 5
Acq On : 28-May-2013, 11:58 Operator: QM
Sample : HSTDICC001 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: May 28 12:51 2013 Quant Results File: HN052813.RES

Instrument :
HPLC_N
LabSampleId :
HSTDICC001

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN052813.M
Title :
Last Update : Tue May 28 12:45:46 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

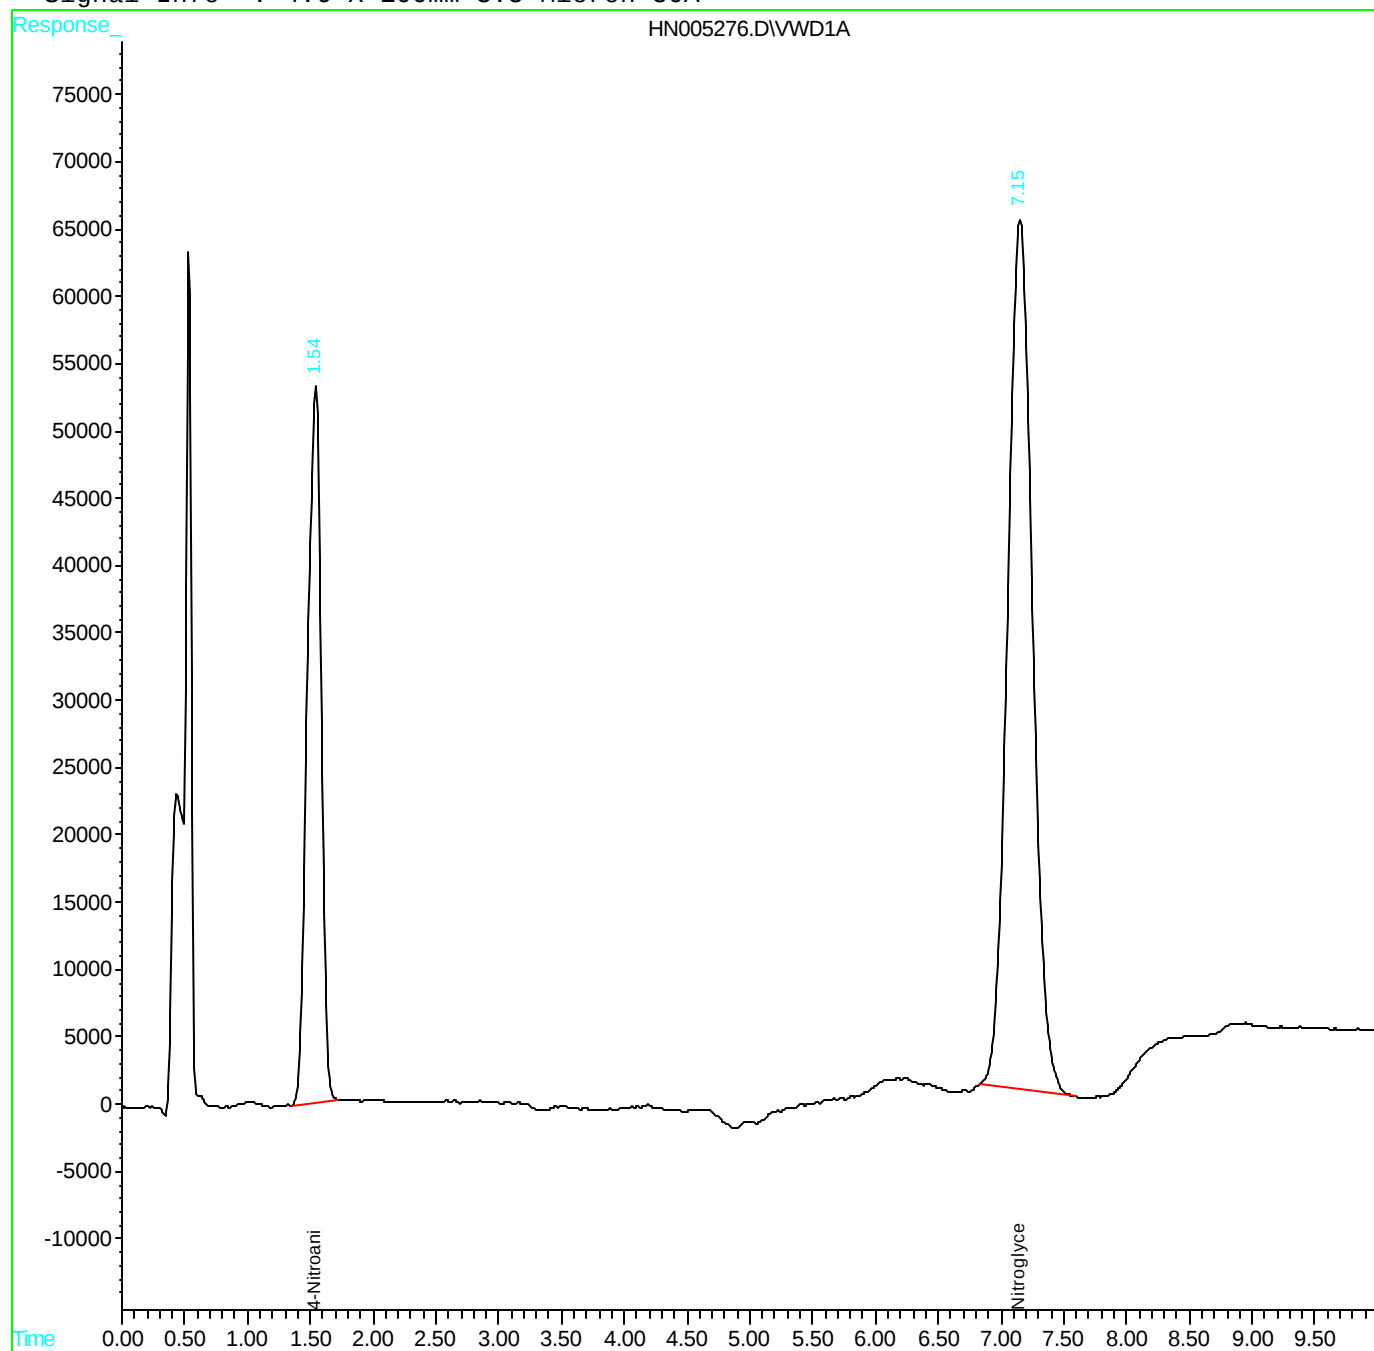


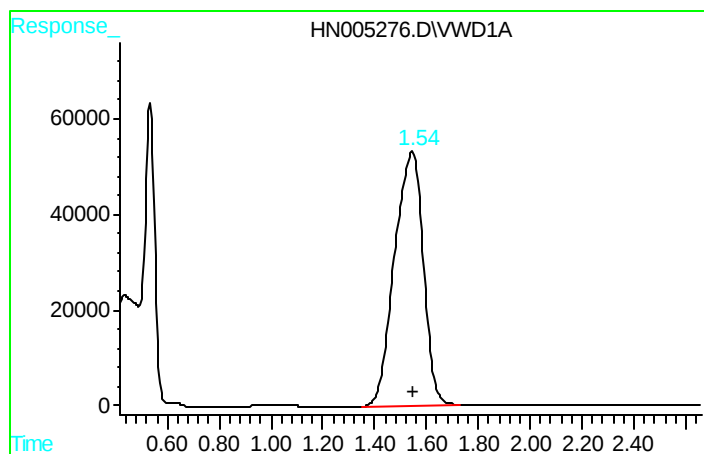

#1 4-Nitroaniline

R.T.: 1.546 min
Delta R.T.: -0.004 min
Response: 4094704
Conc: 0.94 ng/uL

Instrument :
HPLC_N
LabSampleId :
HSTDIC001

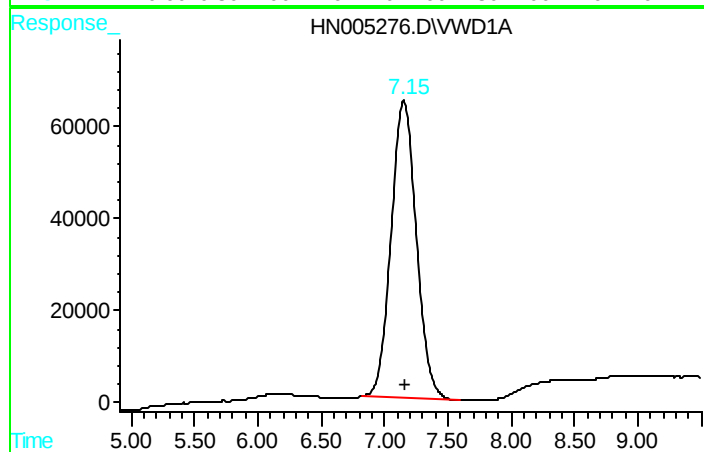

#2 Nitroglycerin

R.T.: 7.153 min
Delta R.T.: -0.003 min
Response: 8928553
Conc: 1.00 ng/uL