

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN052813\HN005277.D Vial: 6
Acq On : 28-May-2013, 12:10 Operator: QM
Sample : HSTDICC0.5 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: May 28 12:51 2013 Quant Results File: HN052813.RES

Instrument :
HPLC_N
LabSampleId :
HSTDICC0.5

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN052813.M
Title :
Last Update : Tue May 28 12:45:46 2013
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.52	2051215	0.470 ng/uL
Target Compounds			
2) T Nitroglycerin	7.21	4298293	0.480 ng/uL

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005277.D HN052813.M

Tue May 28 14:08:05 2013

RPT1


Quantitation Report


Data File : Z:\HPCHEM1\HPLC_N\DATA\HN052813\HN005277.D Vial: 6
Acq On : 28-May-2013, 12:10 Operator: QM
Sample : HSTDICC0.5 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: May 28 12:51 2013 Quant Results File: HN052813.RES

Instrument :
HPLC_N
LabSampleId :
HSTDICC0.5

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN052813.M
Title :
Last Update : Tue May 28 12:45:46 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

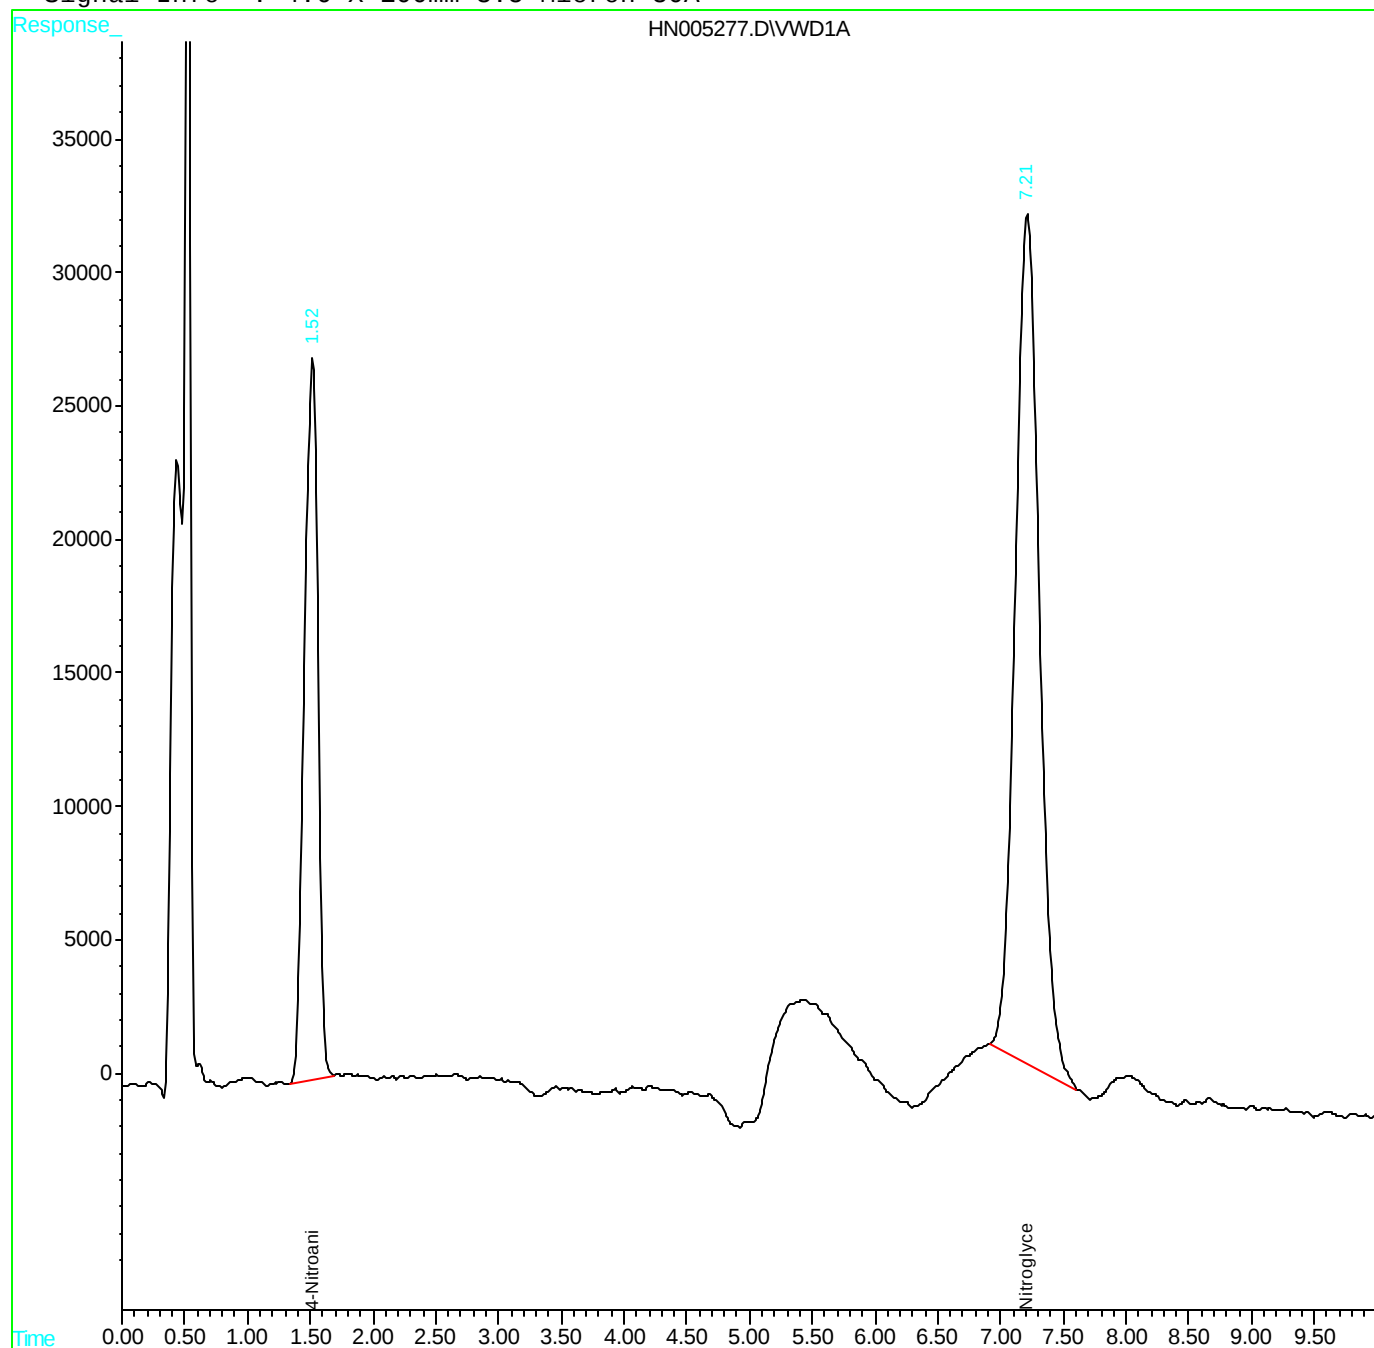


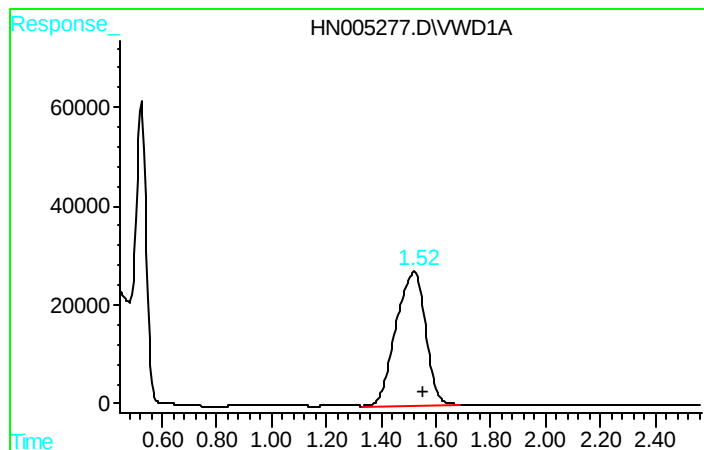

#1 4-Nitroaniline

R.T.: 1.521 min
Delta R.T.: -0.029 min
Response: 2051215
Conc: 0.47 ng/uL

Instrument :
HPLC_N
LabSampleId :
HSTDIC0.5

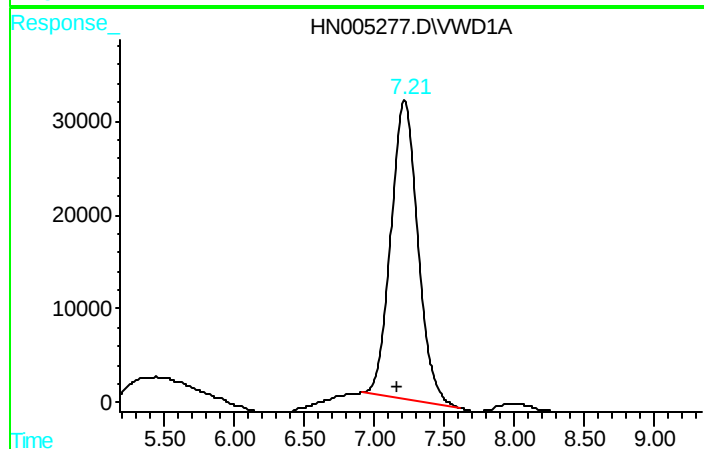

#2 Nitroglycerin

R.T.: 7.213 min
Delta R.T.: 0.057 min
Response: 4298293
Conc: 0.48 ng/uL