

Data File : Z:\HPCHEM1\HPLC\_N\DATA\HN052813\HN005281.D Vial: 3  
 Acq On : 28-May-2013, 13:57 Operator: QM  
 Sample : PB69815BL Inst : G1314A  
 Misc : Multiplr: 1.00  
 IntFile : autoint1.e  
 Quant Time: May 28 14:30 2013 Quant Results File: HN052813.RES

Instrument :  
 HPLC\_N  
 ClientSampleId :  
 PB69815BL

Quant Method : Z:\HPCHEM1\HPLC\_N\METHOD\HN052813.M  
 Title :  
 Last Update : Tue May 28 14:18:38 2013  
 Response via : Initial Calibration  
 DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul  
 Signal Phase : ZORBAX Extend-C18  
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
1) S 4-Nitroaniline	1.54	627422	0.151 ng/uL
Target Compounds			

-----  
 Analyst Signature: \_\_\_\_\_ Analyst Name: \_\_\_\_\_ Date: \_\_\_\_\_  
 -----

-----REASONS FOR MANUAL INTEGRATIONS-----

\_\_\_ Poor resolution of peaks exhibited on chromatogram.Compound #: \_\_\_\_\_

\_\_\_ Peak integrated by software incorrectly.Compound #: \_\_\_\_\_

\_\_\_ OTHER: \_\_\_\_\_ Compound #: \_\_\_\_\_

(f)=RT Delta > 1/2 Window (m)=manual int.


Quantitation Report


Data File : Z:\HPCHEM1\HPLC\_N\DATA\HN052813\HN005281.D Vial: 3  
Acq On : 28-May-2013, 13:57 Operator: QM  
Sample : PB69815BL Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : autoint1.e  
Quant Time: May 28 14:30 2013 Quant Results File: HN052813.RES

Instrument :  
HPLC\_N  
ClientSampled :  
PB69815BL

Quant Method : Z:\HPCHEM1\HPLC\_N\METHOD\HN052813.M  
Title :  
Last Update : Tue May 28 14:18:38 2013  
Response via : Multiple Level Calibration  
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

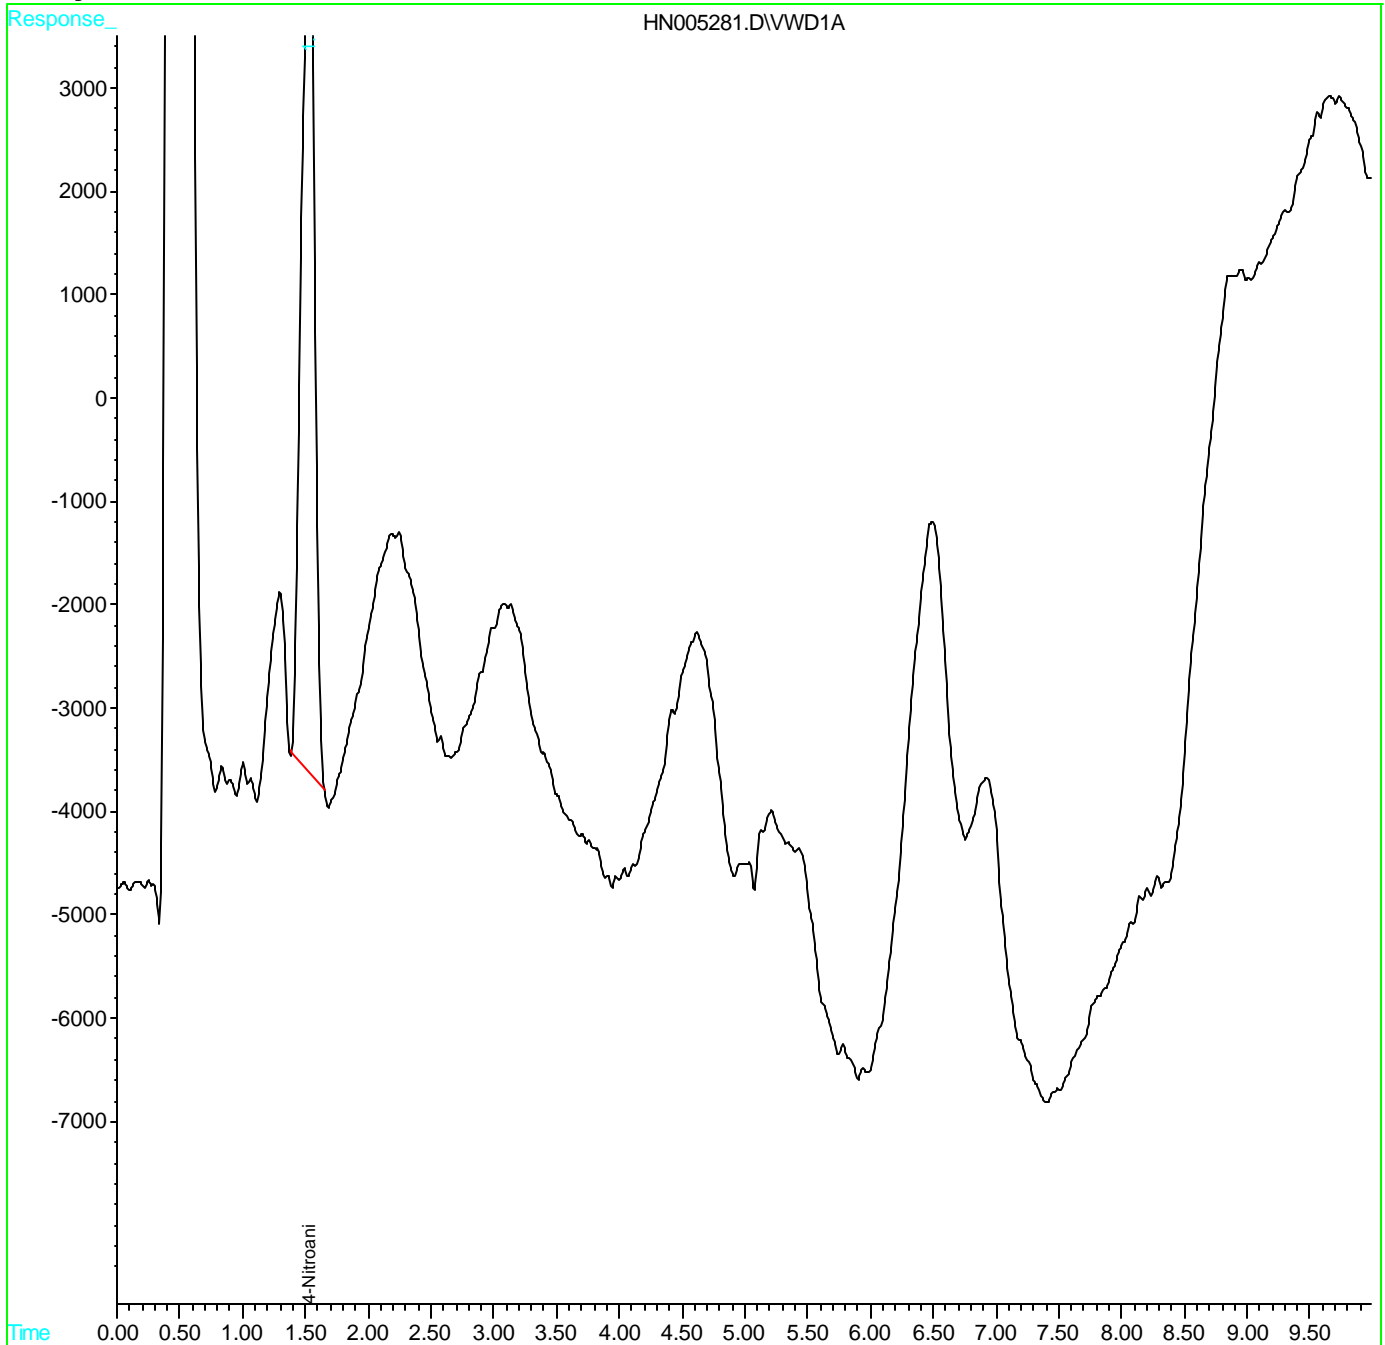

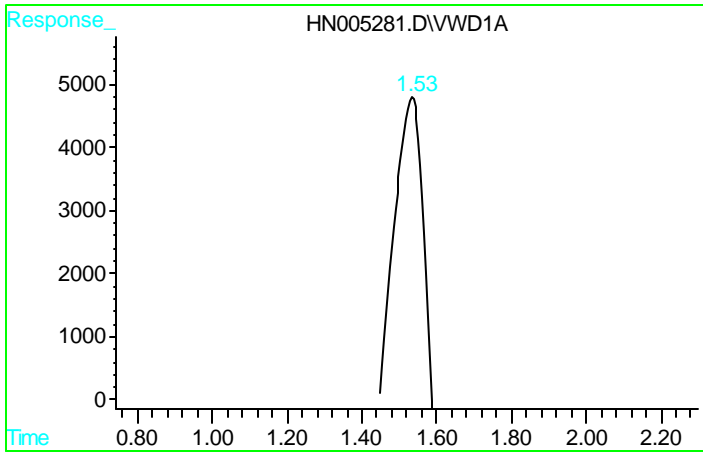

#1 4-Nitroaniline

R.T.: 1.536 min  
Delta R.T.: -0.024 min  
Response: 627422  
Conc: 0.15 ng/uL

Instrument :  
HPLC\_N  
ClientSampled :  
PB69815BL