

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN052813\HN005289.D Vial: 11
Acq On : 28-May-2013, 15:33 Operator: QM
Sample : PB69788BS Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: May 28 15:48 2013 Quant Results File: HN052813.RES

Instrument :
HPLC_N
ClientSampleId :
PB69788BS

Manual Integrations
APPROVED

mohammad
5/31/2013 5:17:02 PM

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN052813.M
Title :
Last Update : Tue May 28 14:18:38 2013
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.57	1442106	0.348 ng/uL m

Target Compounds

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005289.D HN052813.M Tue May 28 15:49:24 2013 RPT1

Quantitation Report

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN052813\HN005289.D Vial: 11
Acq On : 28-May-2013, 15:33 Operator: QM
Sample : PB69788BS Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: May 28 15:48 2013 Quant Results File: HN052813.RES


Instrument :
HPLC_N
ClientSampleId :
PB69788BS


Manual Integrations
APPROVED

mohammad
5/31/2013 5:17:02 PM

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN052813.M
Title :
Last Update : Tue May 28 14:18:38 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

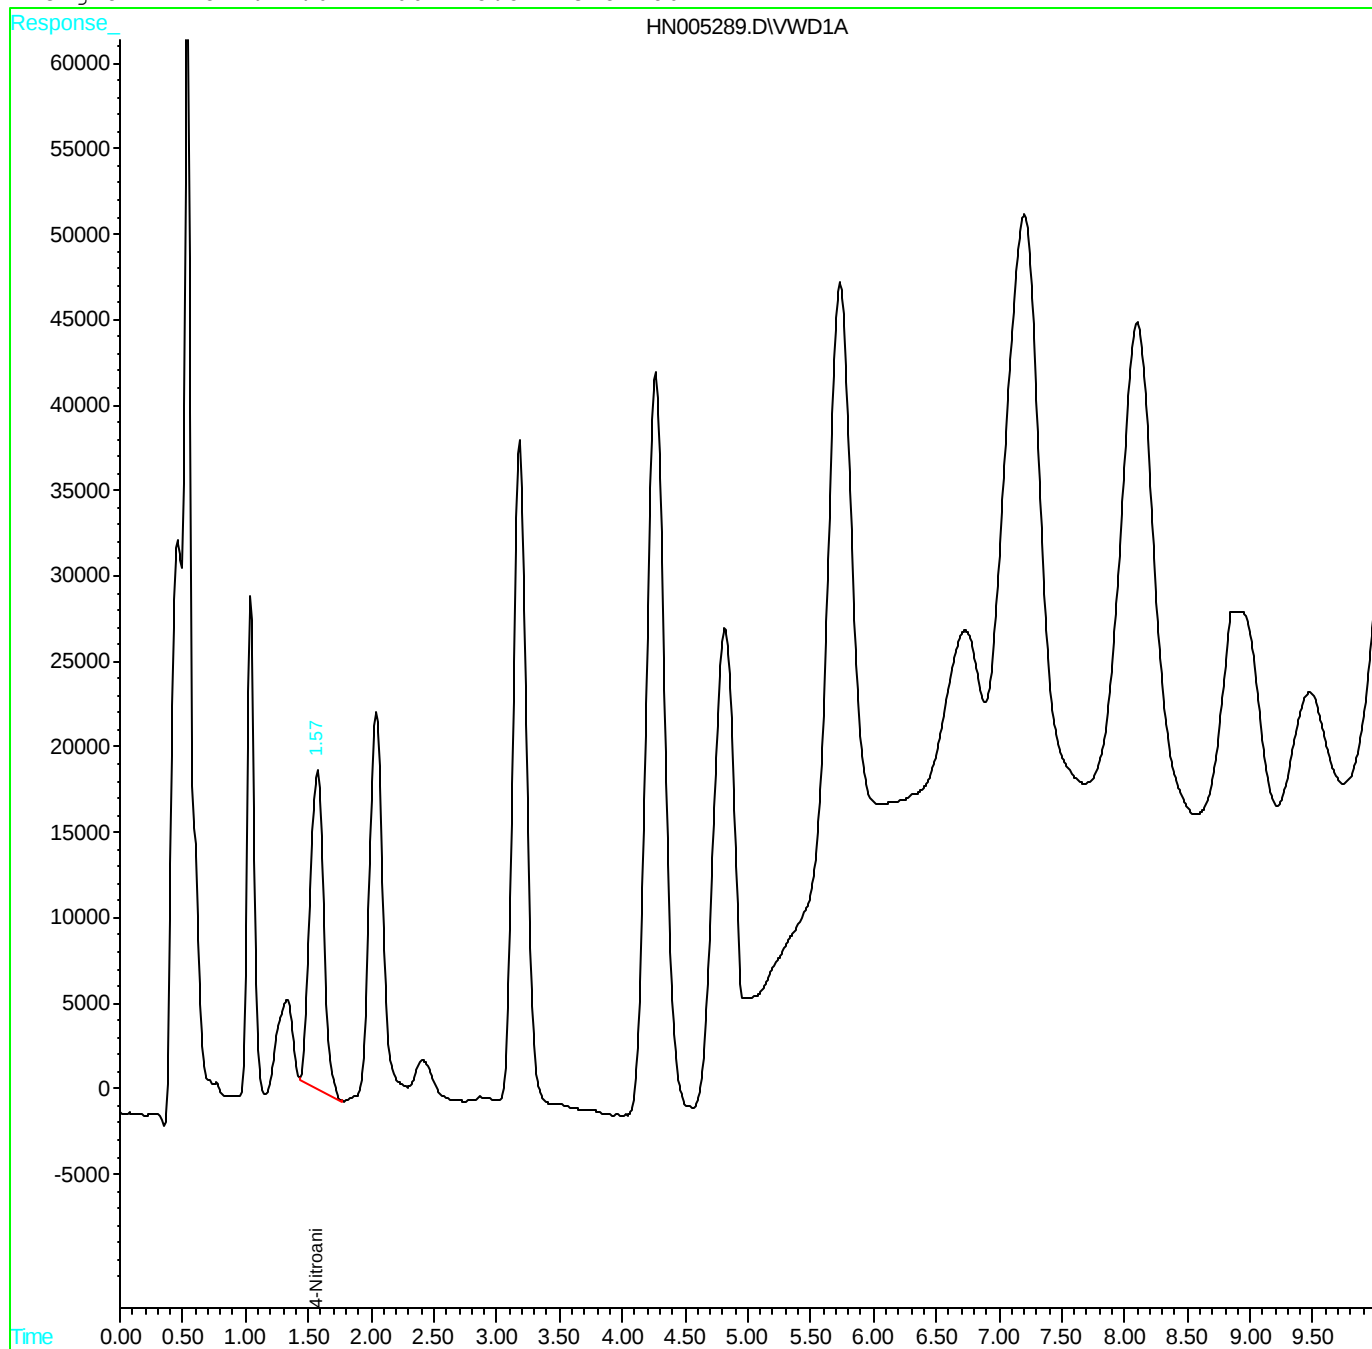

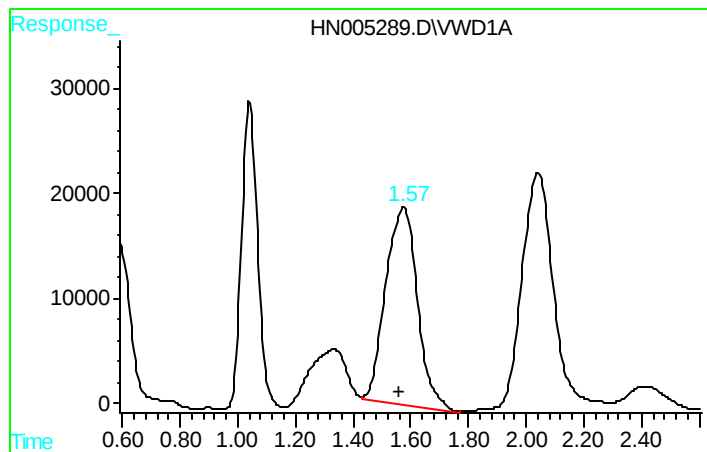

#1 4-Nitroaniline

R.T.: 1.574 min
Delta R.T.: 0.014 min
Response: 1442106
Conc: 0.35 ng/uL

Instrument :

HPLC_N

ClientSampleId :

PB69788BS

Manual Integrations
APPROVED

mohammad
5/31/2013 5:17:02 PM