

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN053113\HN005355.D Vial: 32
Acq On : 31-May-2013, 14:08 Operator: QM
Sample : E2386-01MSD Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: May 31 14:27 2013 Quant Results File: HN052813.RES

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN052813.M
Title :
Last Update : Fri May 31 12:17:10 2013
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.46	831052	0.201 ng/ul
Target Compounds			

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.


HN005355.D HN052813.M Fri May 31 14:27:03 2013 RPT1


Quantitation Report

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN053113\HN005355.D Vial: 32
Acq On : 31-May-2013, 14:08 Operator: QM
Sample : E2386-01MSD Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: May 31 14:27 2013 Quant Results File: HN052813.RES

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN052813.M
Title :
Last Update : Fri May 31 12:17:10 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

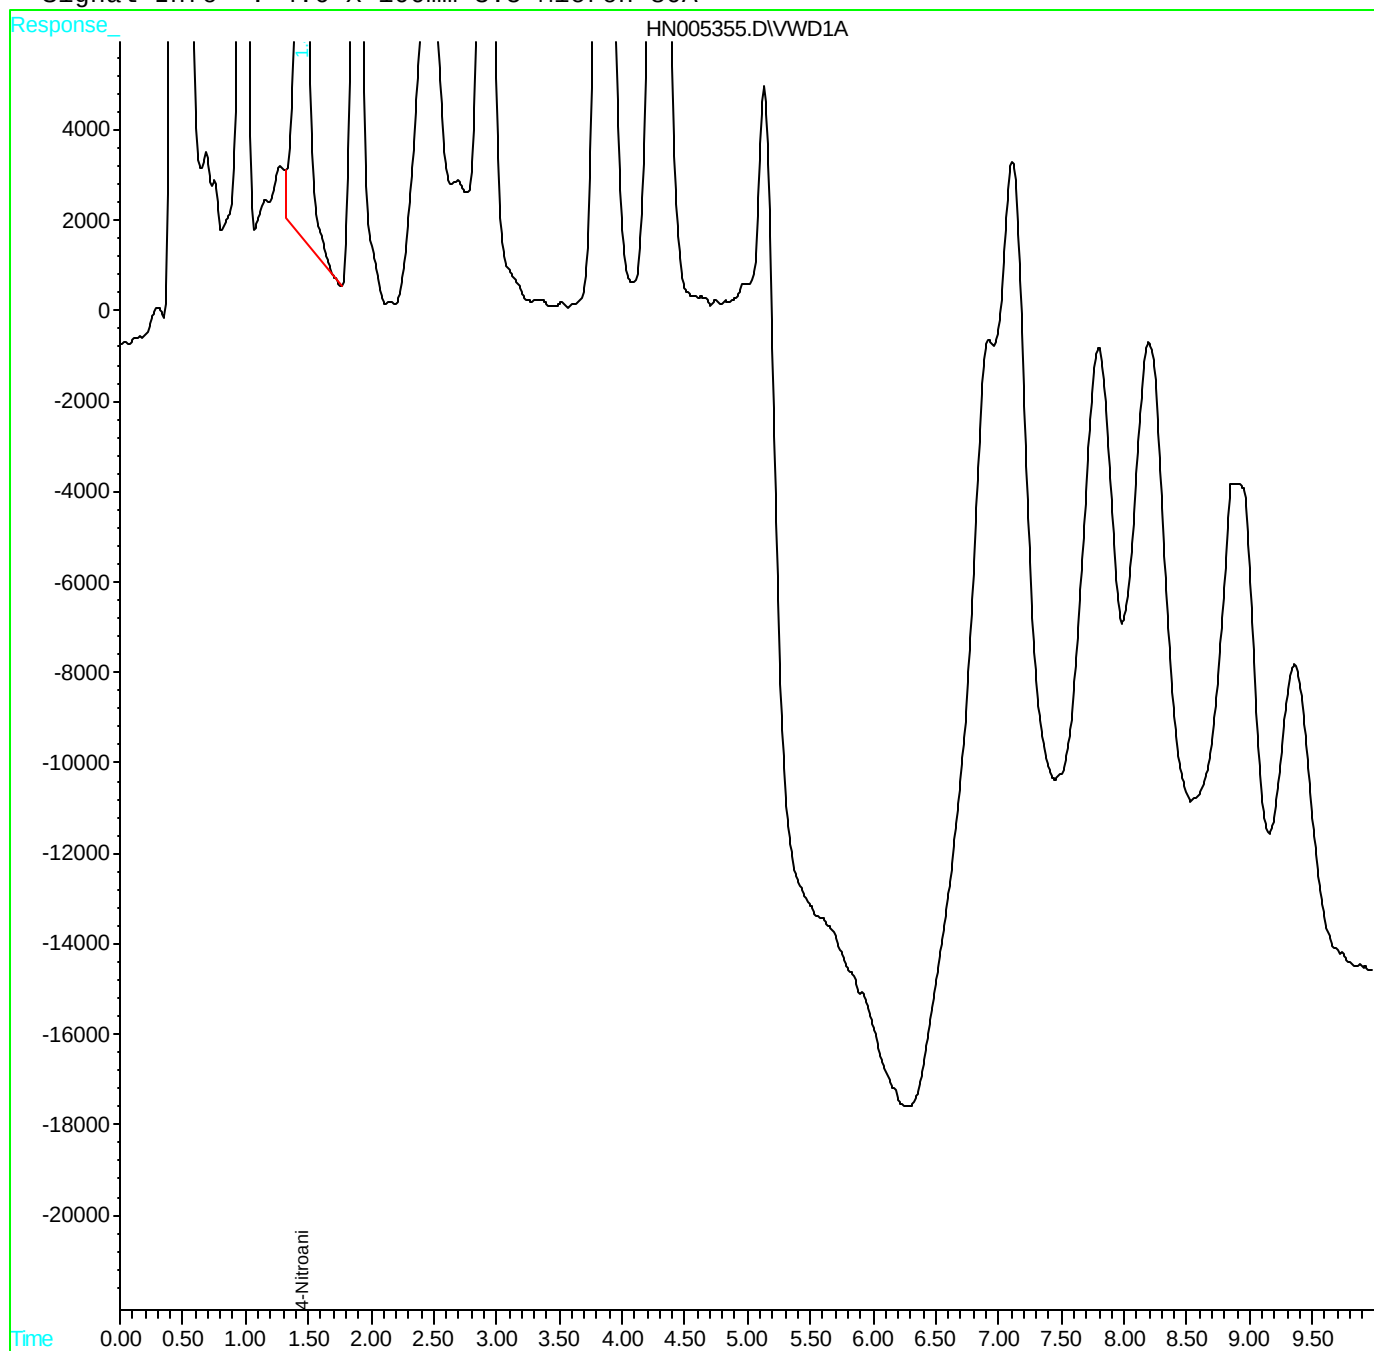

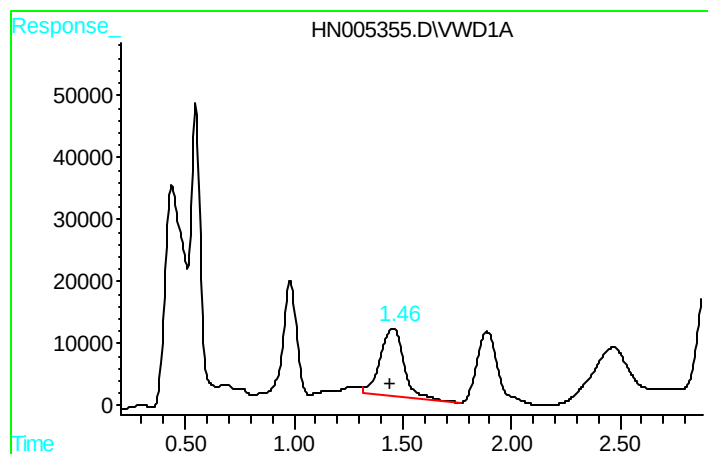

#1 4-Nitroaniline

R.T.: 1.457 min
Delta R.T.: 0.017 min
Response: 831052
Conc: 0.20 ng/ul