

Data File : Z:\HPCHEM1\HPLC\_N\DATA\HN060313\HN005357.D Vial: 31  
Acq On : 03-Jun-2013, 11:39 Operator: QM  
Sample : HSTDCCC005 Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : autoint1.e  
Quant Time: Jun 3 12:15 2013 Quant Results File: HN052813.RES

Instrument :  
HPLC\_N  
LabSampleId :  
HSTDCCC005

Quant Method : Z:\HPCHEM1\HPLC\_N\METHOD\HN052813.M  
Title :  
Last Update : Mon Jun 03 12:15:51 2013  
Response via : Initial Calibration  
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

| Compound                    | R.T. | Response | Conc Units  |
|-----------------------------|------|----------|-------------|
| -----                       |      |          |             |
| System Monitoring Compounds |      |          |             |
| 1) S 4-Nitroaniline         | 1.49 | 21180232 | 5.112 ng/ul |
| Target Compounds            |      |          |             |
| 2) T Nitroglycerin          | 6.93 | 45746416 | 5.221 ng/ul |

-----  
Analyst Signature:\_\_\_\_\_ Analyst Name:\_\_\_\_\_ Date:\_\_\_\_\_

-----REASONS FOR MANUAL INTEGRATIONS-----

\_\_\_Poor resolution of peaks exhibited on chromatogram.Compound #:\_\_\_\_\_

\_\_\_Peak Integrated by software incorrectly.Compound #:\_\_\_\_\_

\_\_\_OTHER:\_\_\_\_\_Compound #:\_\_\_\_\_

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005357.D HN052813.M

Mon Jun 03 15:57:20 2013

RPT1


# Quantitation Report


Data File : Z:\HPCHEM1\HPLC\_N\DATA\HN060313\HN005357.D Vial: 31  
Acq On : 03-Jun-2013, 11:39 Operator: QM  
Sample : HSTDCCC005 Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : autoint1.e  
Quant Time: Jun 3 12:15 2013 Quant Results File: HN052813.RES

Instrument :  
HPLC\_N  
LabSampleId :  
HSTDCCC005

Quant Method : Z:\HPCHEM1\HPLC\_N\METHOD\HN052813.M  
Title :  
Last Update : Mon Jun 03 12:15:51 2013  
Response via : Multiple Level Calibration  
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

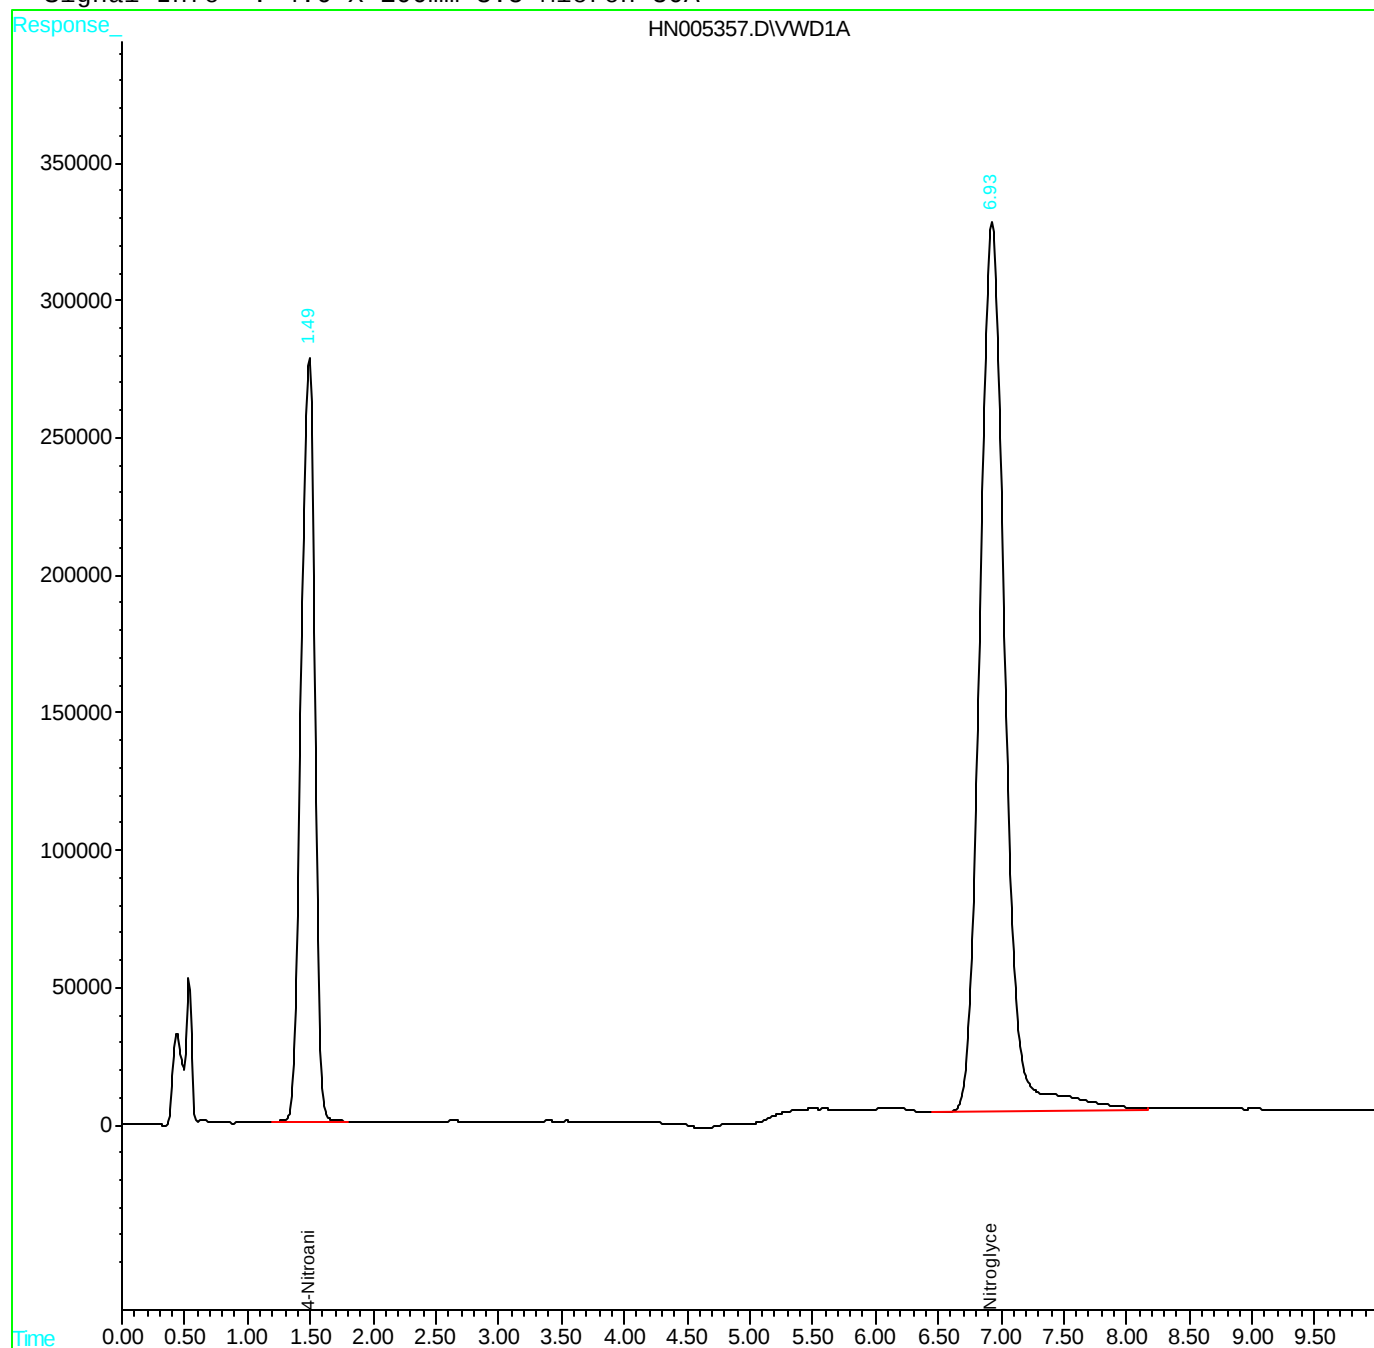


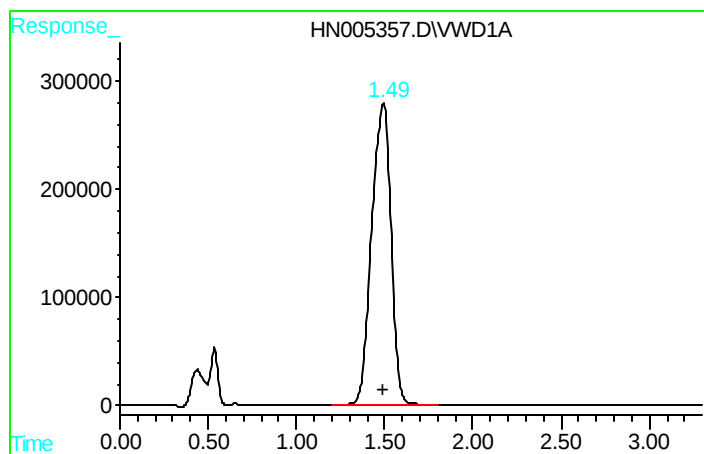

#1 4-Nitroaniline

R.T.: 1.494 min  
Delta R.T.: 0.004 min  
Response: 21180232  
Conc: 5.11 ng/ul

Instrument :  
HPLC\_N  
LabSampleId :  
HSTDCCC005

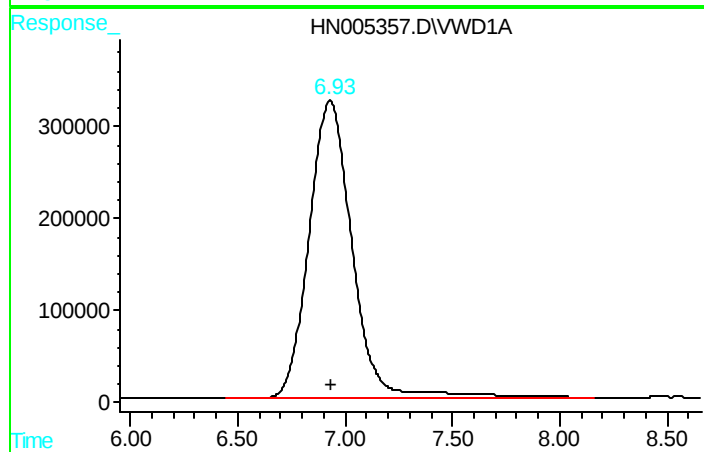

#2 Nitroglycerin

R.T.: 6.930 min  
Delta R.T.: 0.000 min  
Response: 45746416  
Conc: 5.22 ng/ul