

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN060413\HN005366.D Vial: 6
Acq On : 04-Jun-2013, 18:47 Operator: QM
Sample : E2428-01 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jun 5 11:00 2013 Quant Results File: HN052813.RES

Instrument :
HPLC_N
ClientSampleId :
SS26-WC15

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN052813.M
Title :
Last Update : Wed Jun 05 10:59:35 2013
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
2) T Nitroglycerin	6.87	3463	0.000 ng/ul

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005366.D HN052813.M

Wed Jun 05 11:00:46 2013

RPT1


Quantitation Report


Data File : Z:\HPCHEM1\HPLC_N\DATA\HN060413\HN005366.D Vial: 6
Acq On : 04-Jun-2013, 18:47 Operator: QM
Sample : E2428-01 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jun 5 11:00 2013 Quant Results File: HN052813.RES

Instrument :
HPLC_N
ClientSampleId :
SS26-WC15

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN052813.M
Title :
Last Update : Wed Jun 05 10:59:35 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

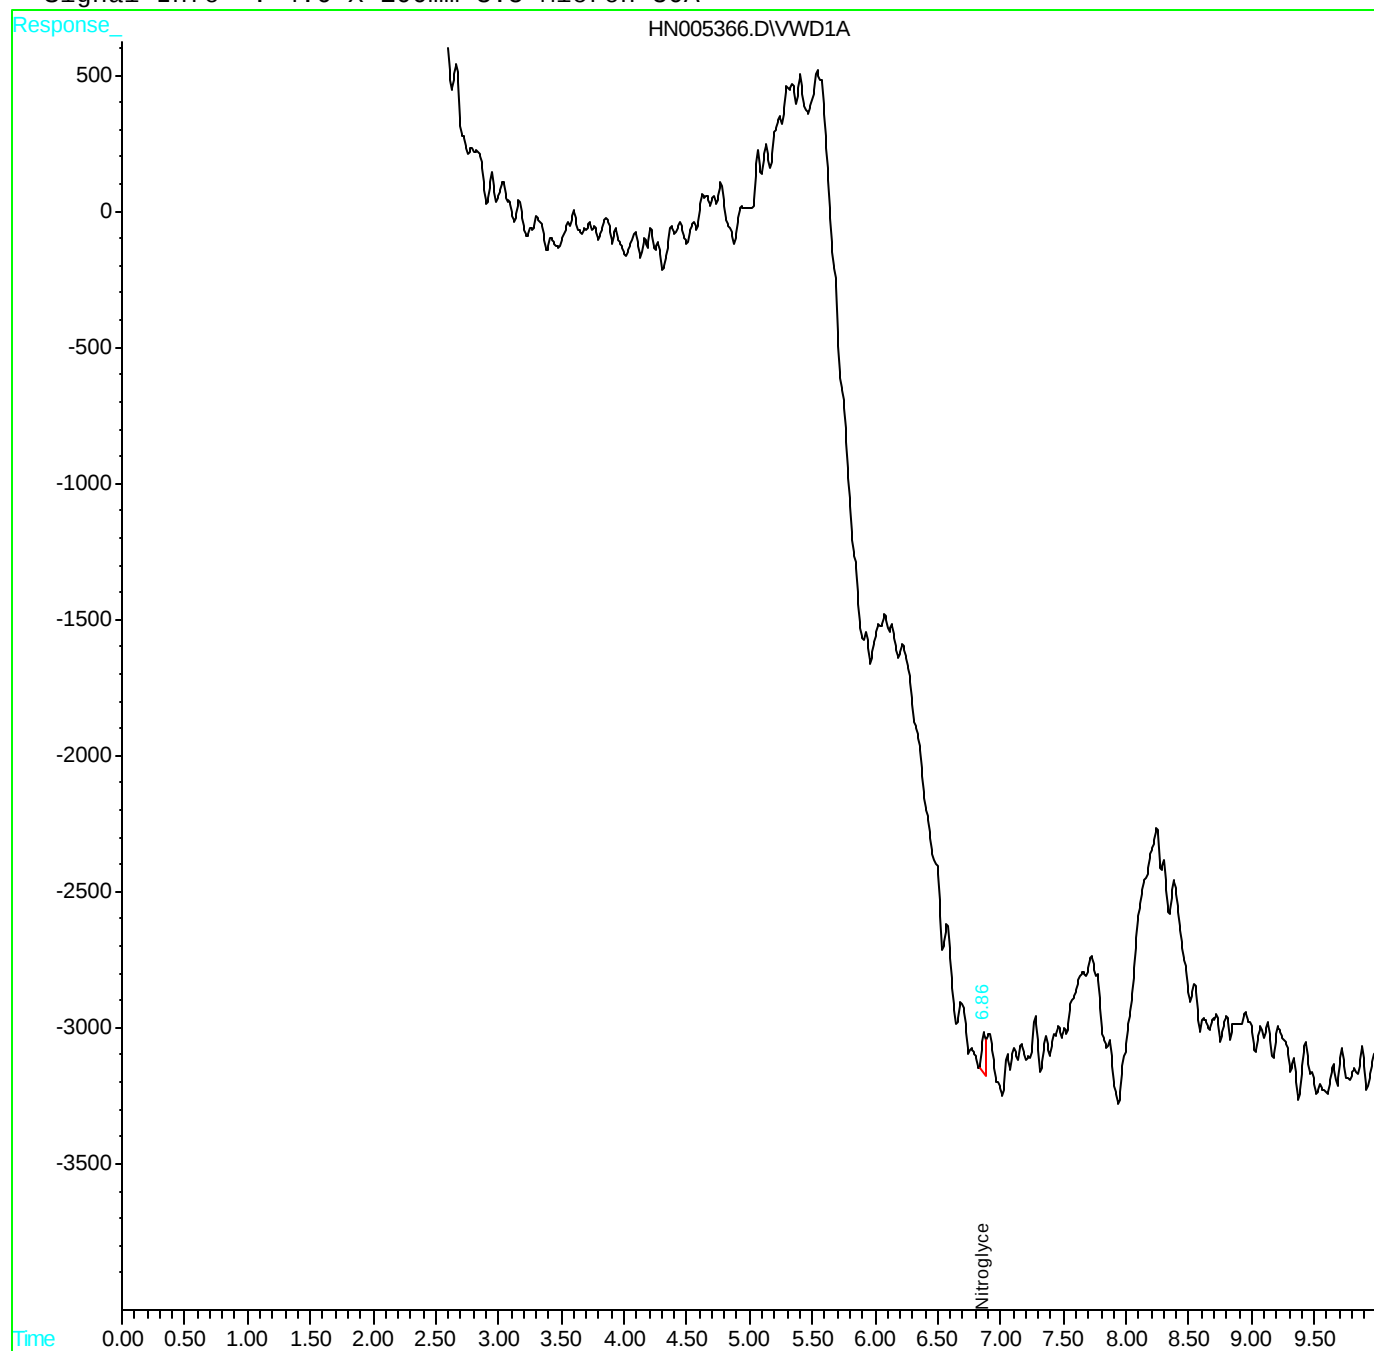


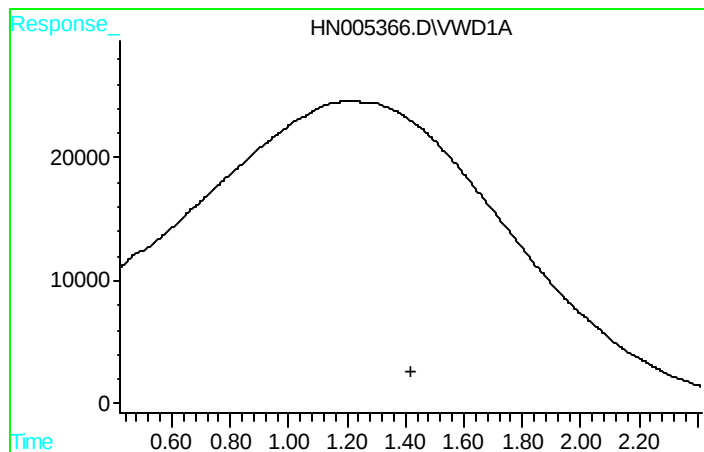

#1 4-Nitroaniline

R.T.: 0.000 min
 Exp R.T.: 1.420 min
 Response: 0
 Conc: N.D.

Instrument :
 HPLC_N
 ClientSampleId :
 SS26-WC15

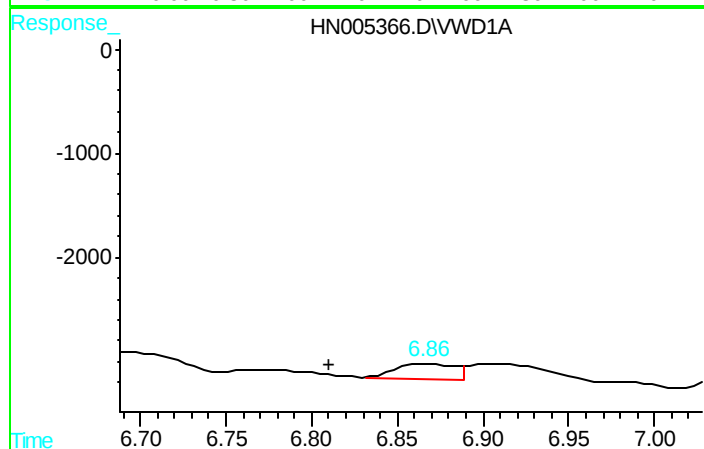

#2 Nitroglycerin

R.T.: 6.868 min
 Delta R.T.: 0.058 min
 Response: 3463
 Conc: 0.00 ng/ul