

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN060413\HN005367.D Vial: 7
Acq On : 04-Jun-2013, 18:59 Operator: QM
Sample : E2428-01MS Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jun 5 11:04 2013 Quant Results File: HN052813.RES

Instrument :
HPLC_N
ClientSampleId :
SS26-WC15MS

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN052813.M
Title :
Last Update : Wed Jun 05 10:59:35 2013
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.37	795644	0.192 ng/ul

Target Compounds

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005367.D HN052813.M

Wed Jun 05 11:04:01 2013

RPT1


Quantitation Report


Data File : Z:\HPCHEM1\HPLC_N\DATA\HN060413\HN005367.D Vial: 7
Acq On : 04-Jun-2013, 18:59 Operator: QM
Sample : E2428-01MS Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jun 5 11:04 2013 Quant Results File: HN052813.RES

Instrument :
HPLC_N
ClientSampleId :
SS26-WC15MS

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN052813.M
Title :
Last Update : Wed Jun 05 10:59:35 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

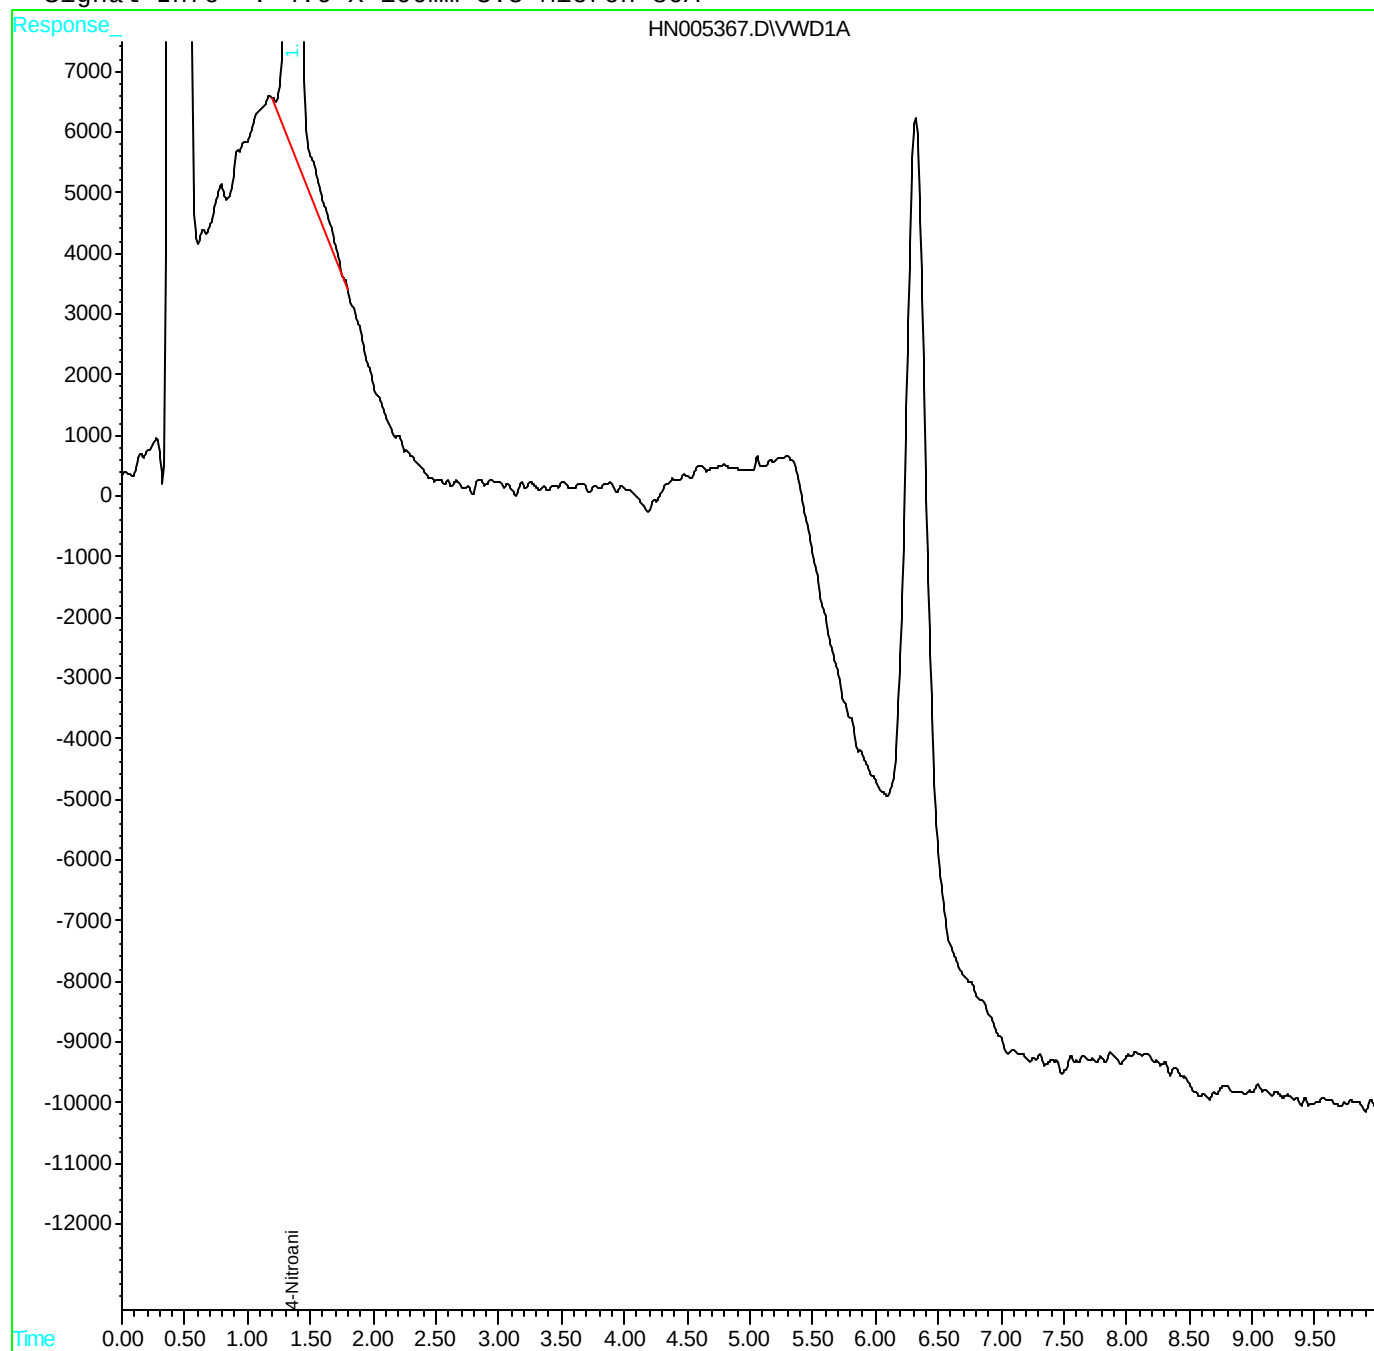

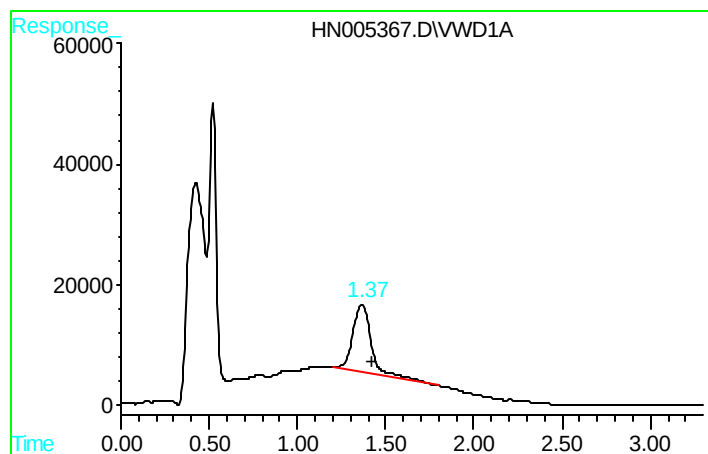

#1 4-Nitroaniline

R.T.: 1.369 min
Delta R.T.: -0.051 min
Response: 795644
Conc: 0.19 ng/ul

Instrument :
HPLC_N
ClientSampleId :
SS26-WC15MS