

Data File : Z:\HPCHEM1\HPLC\_N\DATA\HN060413\HN005375.D Vial: 14  
Acq On : 04-Jun-2013, 20:36 Operator: QM  
Sample : E2197-02 Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : autoint1.e  
Quant Time: Jun 5 11:28 2013 Quant Results File: HN052813.RES

Instrument :  
HPLC\_N  
ClientSampleId :  
B1222SD-02

Quant Method : Z:\HPCHEM1\HPLC\_N\METHOD\HN052813.M  
Title :  
Last Update : Wed Jun 05 11:24:05 2013  
Response via : Initial Calibration  
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

| Compound                    | R.T. | Response | Conc Units  |
|-----------------------------|------|----------|-------------|
| -----                       |      |          |             |
| System Monitoring Compounds |      |          |             |
| 1) S 4-Nitroaniline         | 1.41 | 720544   | 0.174 ng/ul |
| Target Compounds            |      |          |             |
| 2) T Nitroglycerin          | 6.39 | 59194    | 0.007 ng/ul |

-----  
Analyst Signature:\_\_\_\_\_ Analyst Name:\_\_\_\_\_ Date:\_\_\_\_\_

-----REASONS FOR MANUAL INTEGRATIONS-----

\_\_\_Poor resolution of peaks exhibited on chromatogram.Compound #:\_\_\_\_\_

\_\_\_Peak Integrated by software incorrectly.Compound #:\_\_\_\_\_

\_\_\_OTHER:\_\_\_\_\_Compound #:\_\_\_\_\_

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005375.D HN052813.M

Wed Jun 05 11:28:23 2013

RPT1


# Quantitation Report


Data File : Z:\HPCHEM1\HPLC\_N\DATA\HN060413\HN005375.D Vial: 14  
Acq On : 04-Jun-2013, 20:36 Operator: QM  
Sample : E2197-02 Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : autoint1.e  
Quant Time: Jun 5 11:28 2013 Quant Results File: HN052813.RES

Instrument :  
HPLC\_N  
ClientSampleId :  
B1222SD-02

Quant Method : Z:\HPCHEM1\HPLC\_N\METHOD\HN052813.M  
Title :  
Last Update : Wed Jun 05 11:24:05 2013  
Response via : Multiple Level Calibration  
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

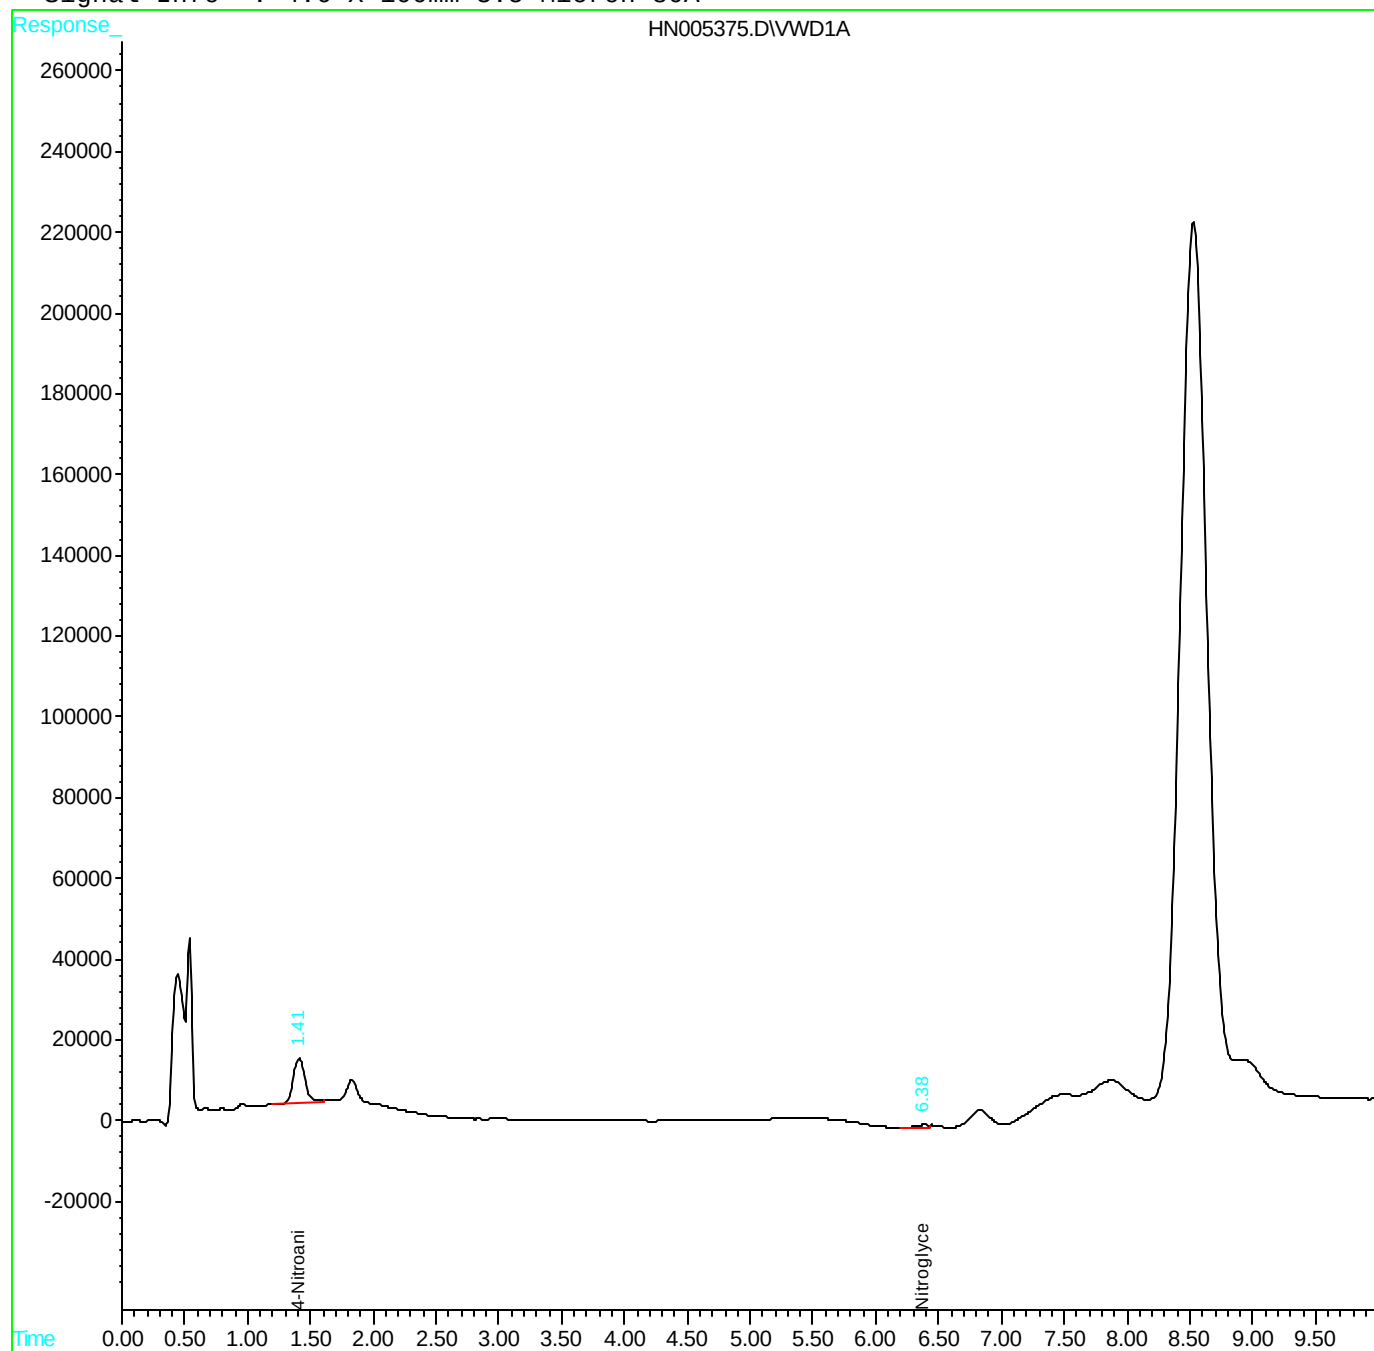


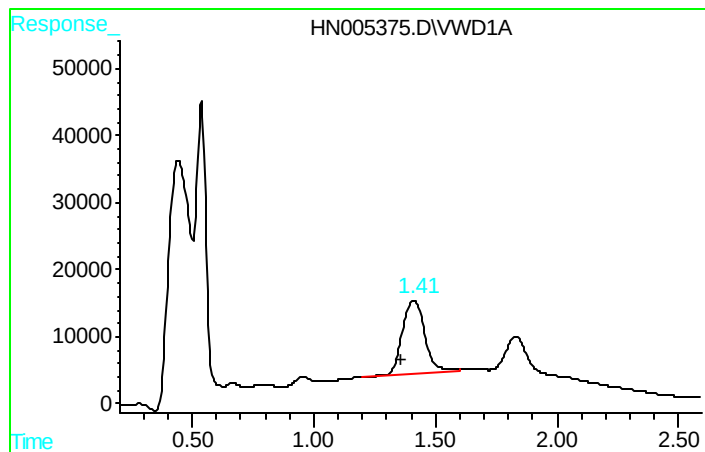

#1 4-Nitroaniline

R.T.: 1.413 min  
 Delta R.T.: 0.053 min  
 Response: 720544  
 Conc: 0.17 ng/ul

Instrument :  
 HPLC\_N  
 ClientSampleId :  
 B1222SD-02

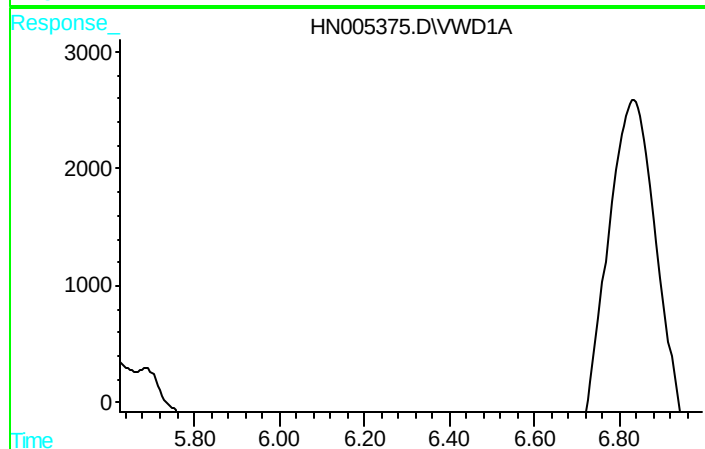

#2 Nitroglycerin

R.T.: 6.385 min  
 Delta R.T.: -0.015 min  
 Response: 59194  
 Conc: 0.01 ng/ul