

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN060413\HN005389.D Vial: 33
 Acq On : 05-Jun-2013, 13:30 Operator: QM
 Sample : E2428-01 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : autoint1.e
 Quant Time: Jun 5 14:08 2013 Quant Results File: HN052813.RES

Instrument :
 HPLC_N
 ClientSampleId :
 SS26-WC15

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN052813.M
 Title :
 Last Update : Wed Jun 05 11:24:05 2013
 Response via : Initial Calibration
 DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.41	666240	0.161 ng/ul

Target Compounds

 Analyst Signature: _____ Analyst Name: _____ Date: _____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #: _____

___Peak Integrated by software incorrectly.Compound #: _____

___OTHER: _____ Compound #: _____

(f)=RT Delta > 1/2 Window (m)=manual int.


Quantitation Report


Data File : Z:\HPCHEM1\HPLC_N\DATA\HN060413\HN005389.D Vial: 33
Acq On : 05-Jun-2013, 13:30 Operator: QM
Sample : E2428-01 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jun 5 14:08 2013 Quant Results File: HN052813.RES

Instrument :
HPLC_N
Client Sampled :
SS26-WC15

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN052813.M
Title :
Last Update : Wed Jun 05 11:24:05 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

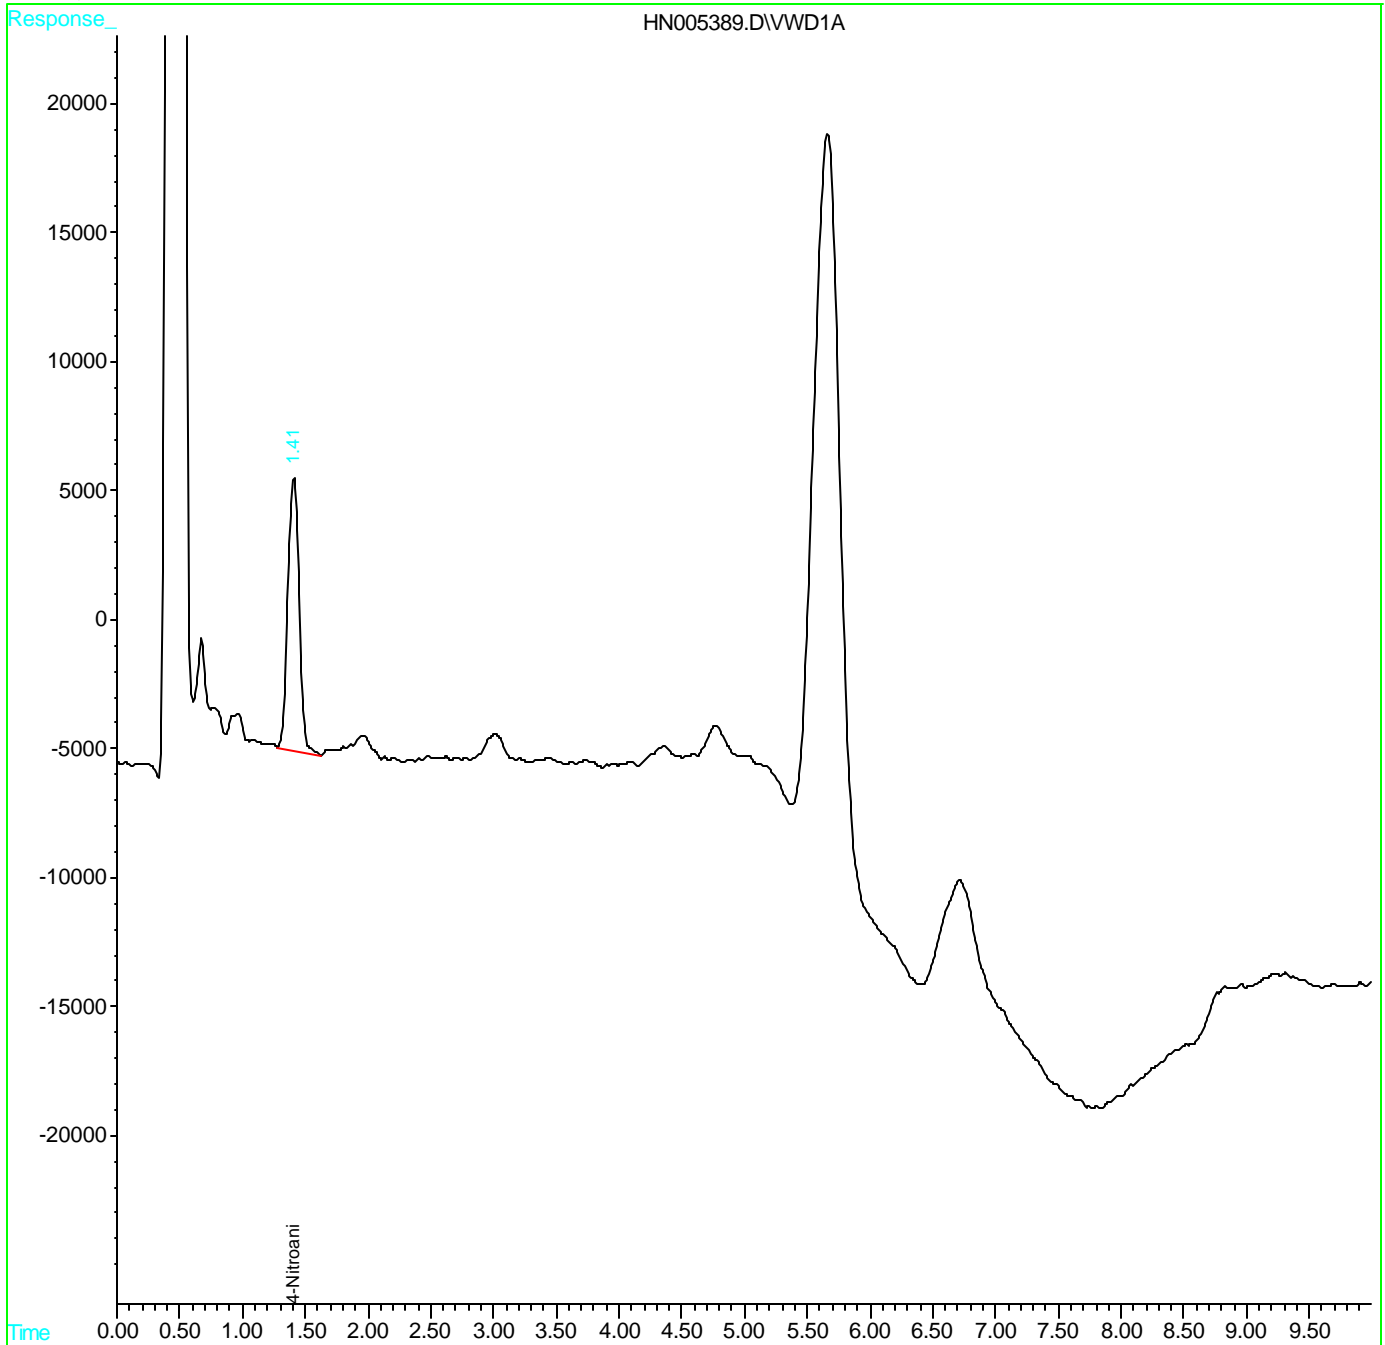

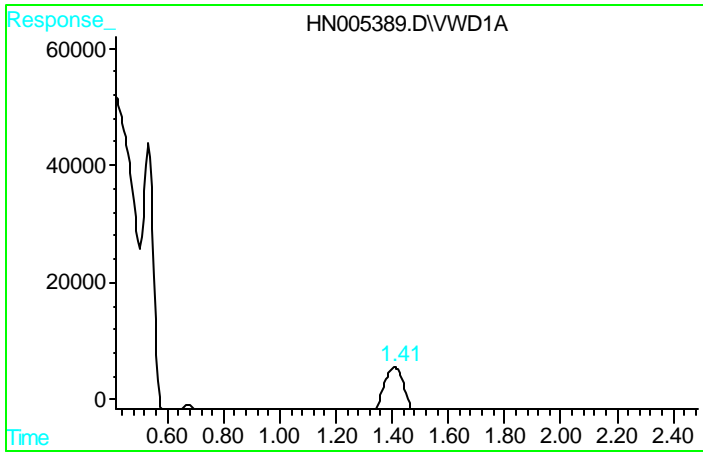

#1 4-Nitroaniline

R.T.: 1.411 min
Delta R.T.: 0.051 min
Response: 666240
Conc: 0.16 ng/ul

Instrument :
HPLC_N
ClientSampled :
SS26-WC15