

Data File : Z:\HPCHEM1\HPLC\_N\DATA\HN060413\HN005390.D Vial: 34  
Acq On : 05-Jun-2013, 14:02 Operator: QM  
Sample : E2428-01MSD Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : autoint1.e  
Quant Time: Jun 5 14:14 2013 Quant Results File: HN052813.RES

Instrument :  
HPLC\_N  
ClientSampleId :  
SS26-WC15MSD

Quant Method : Z:\HPCHEM1\HPLC\_N\METHOD\HN052813.M  
Title :  
Last Update : Wed Jun 05 14:13:58 2013  
Response via : Initial Calibration  
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

| Compound                    | R.T. | Response | Conc Units  |
|-----------------------------|------|----------|-------------|
| -----                       |      |          |             |
| System Monitoring Compounds |      |          |             |
| 1) S 4-Nitroaniline         | 1.49 | 714786   | 0.173 ng/ul |
| Target Compounds            |      |          |             |
| 2) T Nitroglycerin          | 6.56 | 1191239  | 0.136 ng/ul |

-----  
Analyst Signature:\_\_\_\_\_ Analyst Name:\_\_\_\_\_ Date:\_\_\_\_\_

-----REASONS FOR MANUAL INTEGRATIONS-----

\_\_\_Poor resolution of peaks exhibited on chromatogram.Compound #:\_\_\_\_\_

\_\_\_Peak Integrated by software incorrectly.Compound #:\_\_\_\_\_

\_\_\_OTHER:\_\_\_\_\_Compound #:\_\_\_\_\_

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005390.D HN052813.M

Wed Jun 05 14:14:03 2013

RPT1


# Quantitation Report


Data File : Z:\HPCHEM1\HPLC\_N\DATA\HN060413\HN005390.D Vial: 34  
Acq On : 05-Jun-2013, 14:02 Operator: QM  
Sample : E2428-01MSD Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : autoint1.e  
Quant Time: Jun 5 14:14 2013 Quant Results File: HN052813.RES

Instrument :  
HPLC\_N  
ClientSampleId :  
SS26-WC15MSD

Quant Method : Z:\HPCHEM1\HPLC\_N\METHOD\HN052813.M  
Title :  
Last Update : Wed Jun 05 14:13:58 2013  
Response via : Multiple Level Calibration  
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

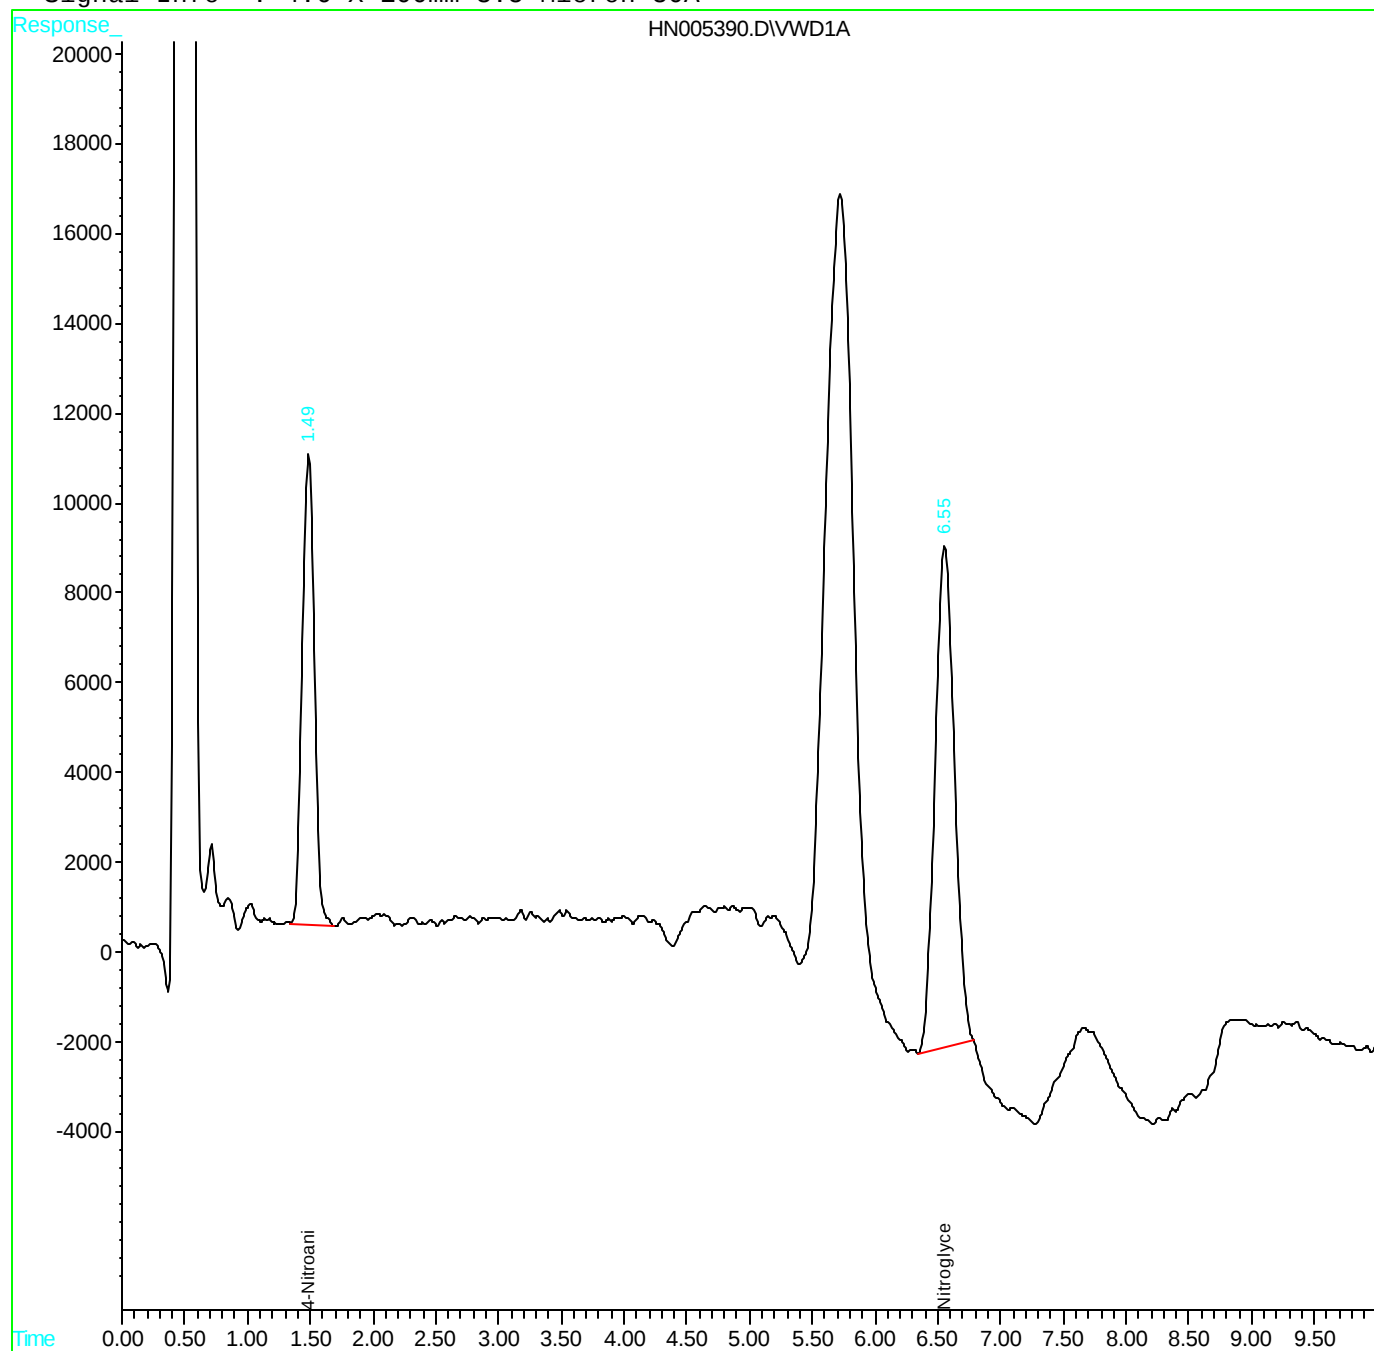


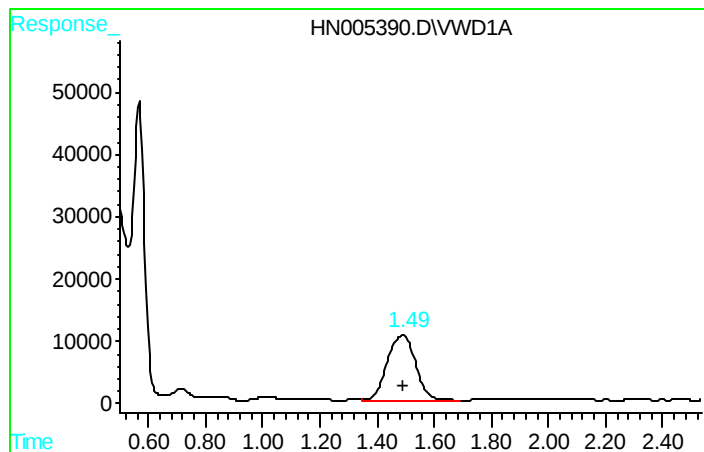

#1 4-Nitroaniline

R.T.: 1.492 min  
 Delta R.T.: 0.002 min  
 Response: 714786  
 Conc: 0.17 ng/ul

Instrument :  
 HPLC\_N  
 ClientSampleId :  
 SS26-WC15MSD

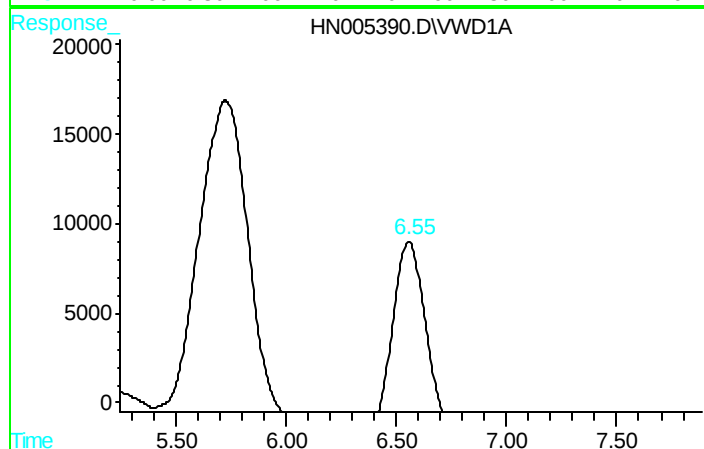

#2 Nitroglycerin

R.T.: 6.555 min  
 Delta R.T.: 0.005 min  
 Response: 1191239  
 Conc: 0.14 ng/ul