

Data Path : Z:\HPCHEM1\HPLC\_N\Data\HN060413\  
Data File : HN005370.D  
Signal(s) : VWD1A.CH  
Acq On : 04-Jun-2013, 19:35  
Operator : QM  
Sample : PB70180BS  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
HPLC\_N  
ClientSampleId :  
PB70180BS

Manual Integrations  
APPROVED

AHPatel  
6/6/2013 2:26:45 AM

Integration File: AUTOINT1.E  
Quant Time: Jun 07 23:30:14 2013  
Quant Method : Z:\HPCHEM1\HPLC\_N\METHOD\HN052813.M  
Quant Title :  
QLast Update : Wed Jun 05 11:06:49 2013  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

| Compound                    | R.T.  | Response | Conc Units   |
|-----------------------------|-------|----------|--------------|
| -----                       |       |          |              |
| System Monitoring Compounds |       |          |              |
| 1) S 4-Nitroaniline         | 1.397 | 743873   | 0.180 ng/ul  |
|                             |       |          |              |
| Target Compounds            |       |          |              |
| 2) T Nitroglycerin          | 6.349 | 1100244  | 0.126 ng/ulm |
| -----                       |       |          |              |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\HPCHEM1\HPLC\_N\Data\HN060413\  
Data File : HN005370.D  
Signal(s) : VWD1A.CH  
Acq On : 04-Jun-2013, 19:35  
Operator : QM  
Sample : PB70180BS  
Misc :  
ALS Vial : 10 Sample Multiplier: 1


Instrument :  
HPLC\_N  
ClientSampleId :  
PB70180BS


Manual Integrations  
APPROVED

AHPatel  
6/6/2013 2:26:45 AM

Integration File: AUTOINT1.E  
Quant Time: Jun 07 23:30:14 2013  
Quant Method : Z:\HPCHEM1\HPLC\_N\METHOD\HN052813.M  
Quant Title :  
QLast Update : Wed Jun 05 11:06:49 2013  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

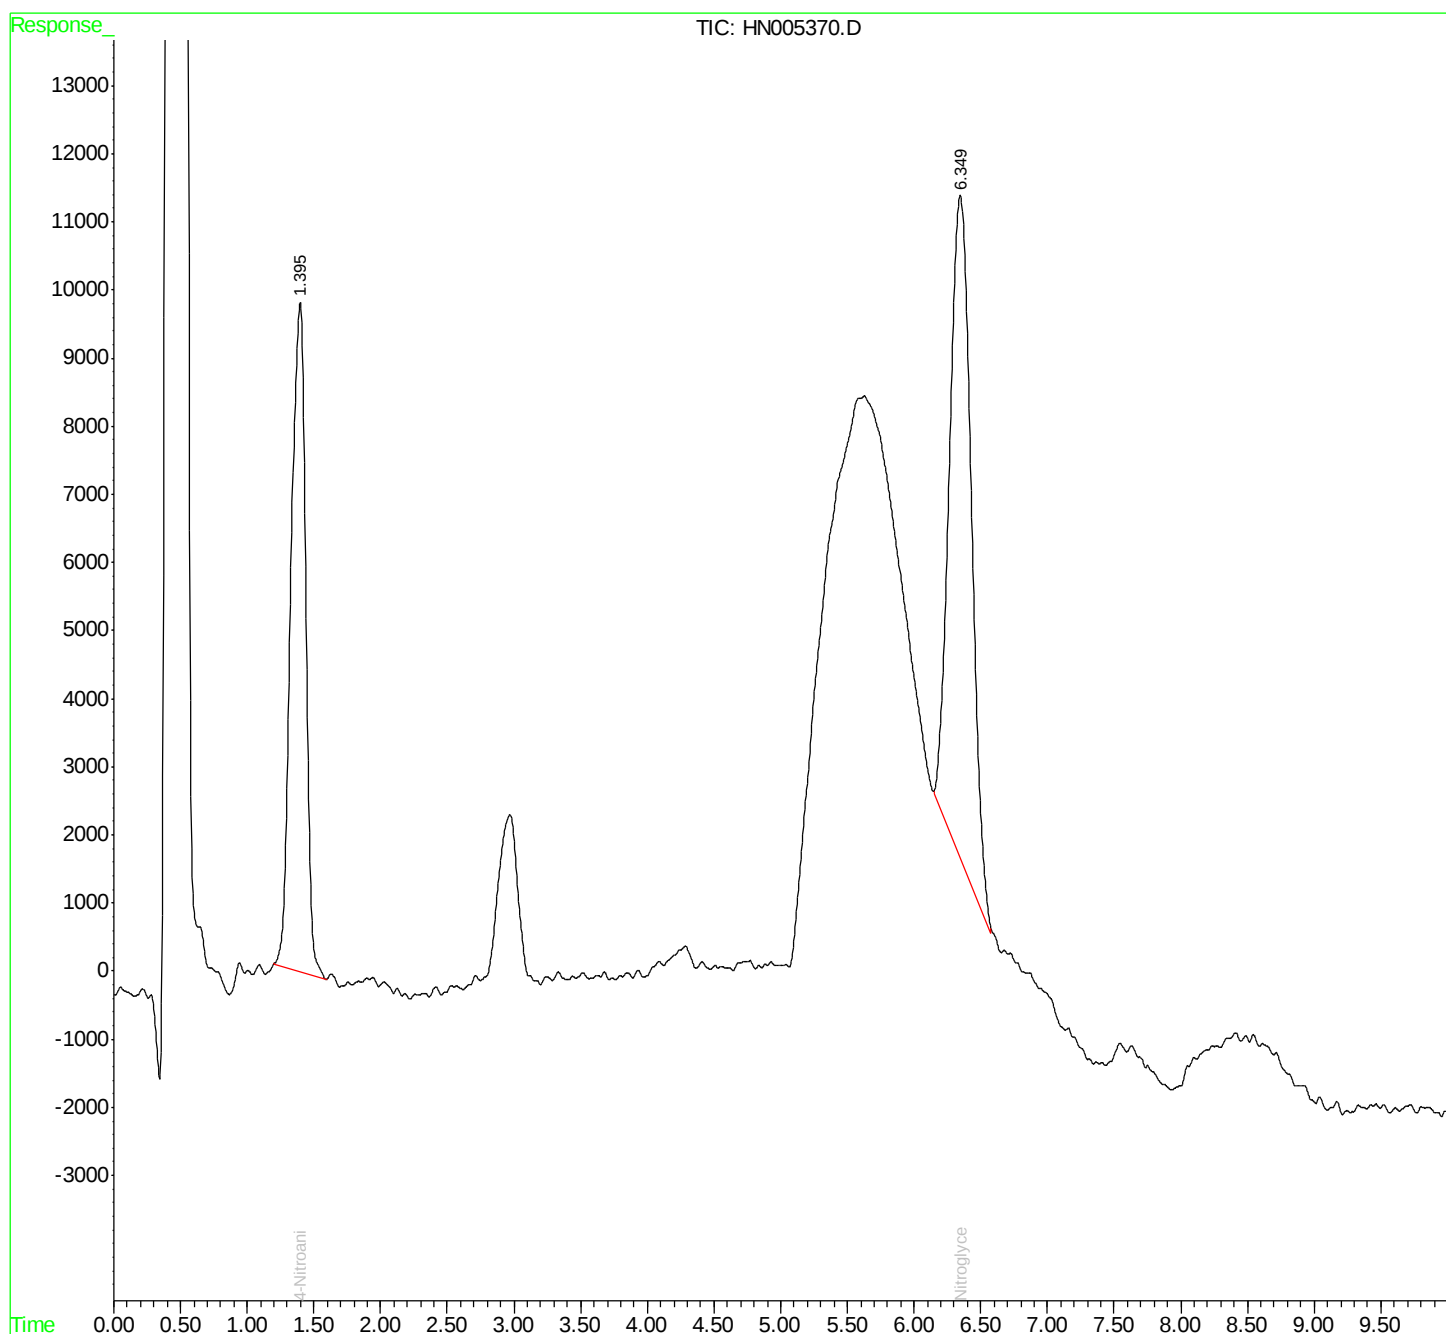

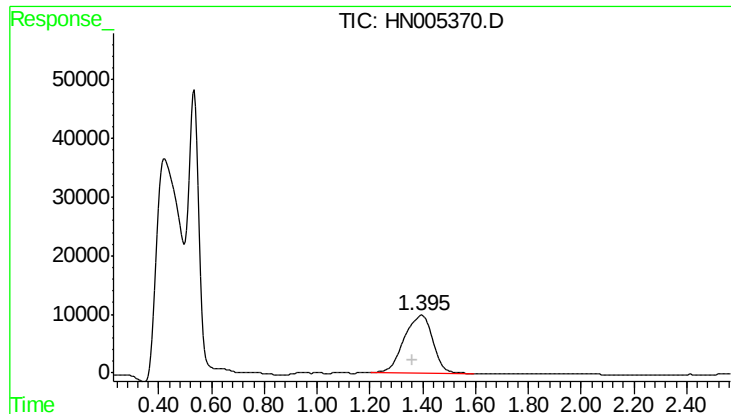


#1 4-Nitroaniline

R.T.: 1.397 min  
Delta R.T.: 0.037 min  
Response: 743873  
Conc: 0.18 ng/u1

Instrument :  
HPLC\_N  
ClientSampleId :  
PB70180BS

Manual Integrations  
APPROVED

AHPatel  
6/6/2013 2:26:45 AM

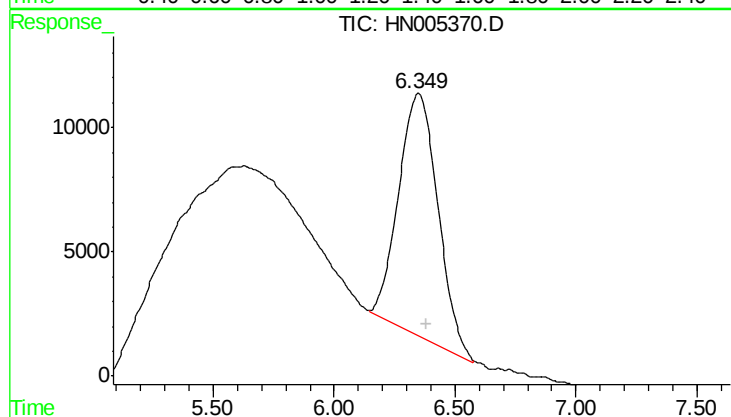

#2 Nitroglycerin

R.T.: 6.349 min  
Delta R.T.: -0.031 min  
Response: 1100244  
Conc: 0.13 ng/u1 m