

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN060913\
Data File : HN005450.D
Signal(s) : VWD1A.CH
Acq On : 09-Jun-2013, 22:55
Operator : QM
Sample : HSTDCCC0500
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
HPLC_N
LabSampleId :
HSTDCCC0500

Integration File: autoint1.e
Quant Time: Jun 10 06:52:54 2013
Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN060913.M
Quant Title :
QLast Update : Mon Jun 10 06:49:47 2013
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	5.483	4867634	426.640 ug/L
Target Compounds			
2) T HMX	4.140	4856201	465.282 ug/L
3) T RDX	6.493	5851150	465.509 ug/L
4) T 1,3,5-Trinitrobenzene	8.903	12064663	482.812 ug/L
9) T 2,4,6-Trinitrotoluene	15.546	9742057	392.755 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN060913\
Data File : HN005450.D
Signal(s) : VWD1A.CH
Acq On : 09-Jun-2013, 22:55
Operator : QM
Sample : HSTDCCC0500
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
HPLC_N
LabSampleId :
HSTDCCC0500

Integration File: autoint1.e
Quant Time: Jun 10 06:52:54 2013
Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN060913.M
Quant Title :
QLast Update : Mon Jun 10 06:49:47 2013
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

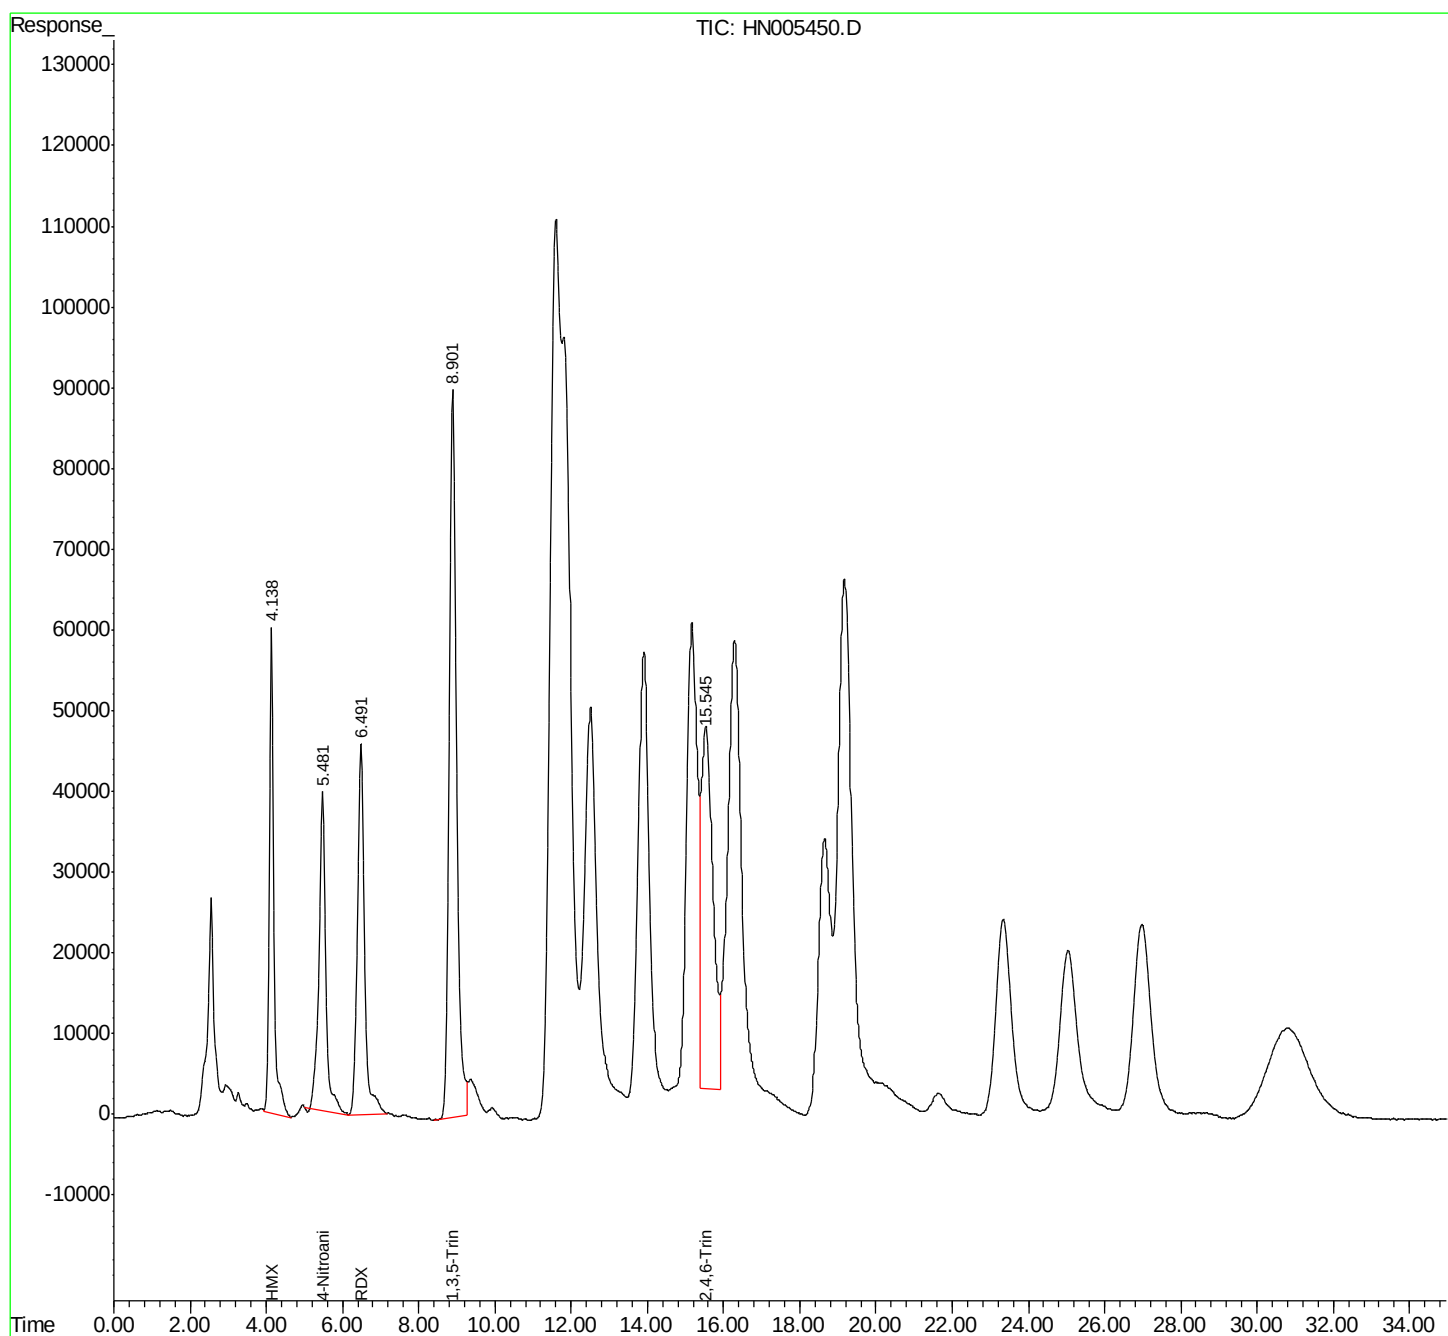


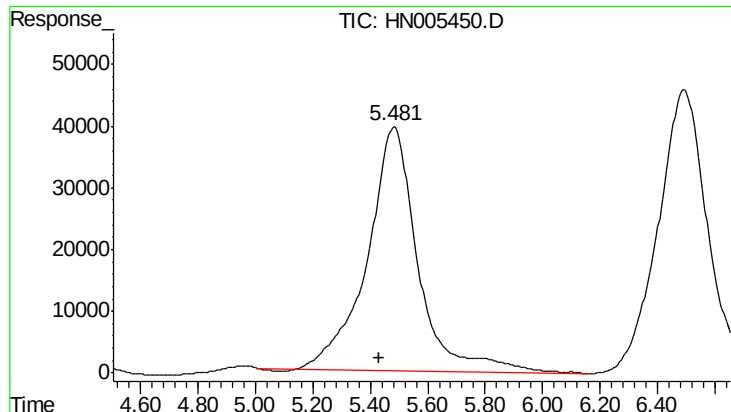

#1 4-Nitroaniline


R.T.: 5.483 min
Delta R.T.: 0.051 min
Response: 4867634
Conc: 426.64 ug/L

Instrument :
HPLC_N
LabSampleId :
HSTDCCC0500

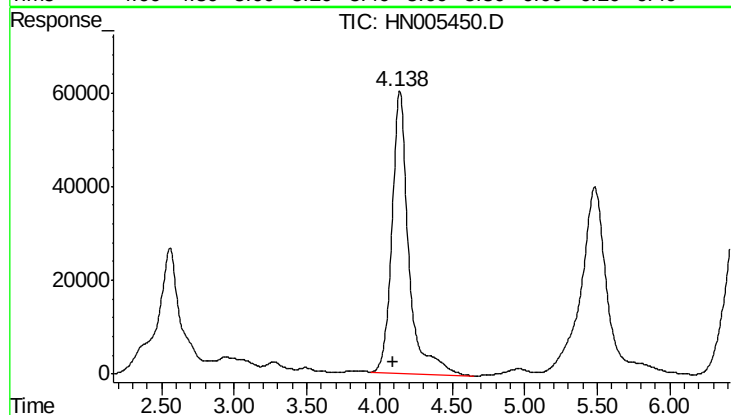


#2 HMX

R.T.: 4.140 min
Delta R.T.: 0.046 min
Response: 4856201
Conc: 465.28 ug/L

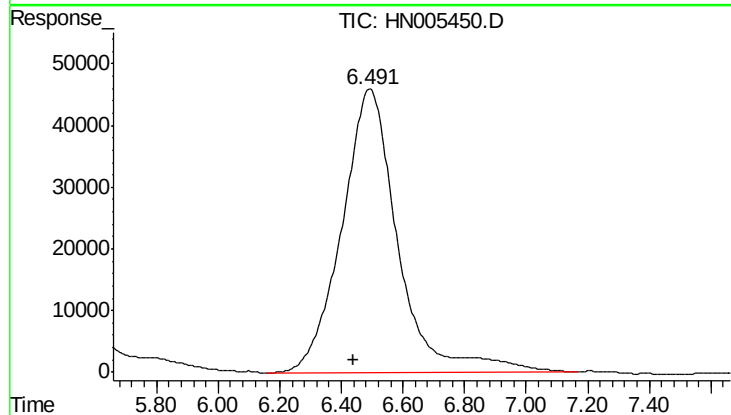


#3 RDX

R.T.: 6.493 min
Delta R.T.: 0.054 min
Response: 5851150
Conc: 465.51 ug/L

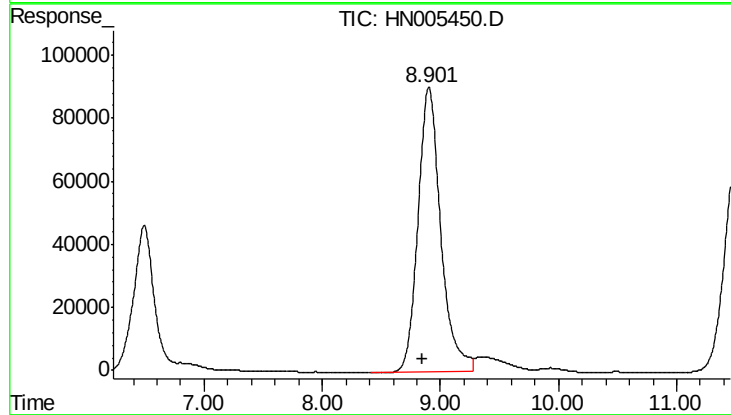

#4 1,3,5-Trinitrobenzene

R.T.: 8.903 min
Delta R.T.: 0.052 min
Response: 12064663
Conc: 482.81 ug/L

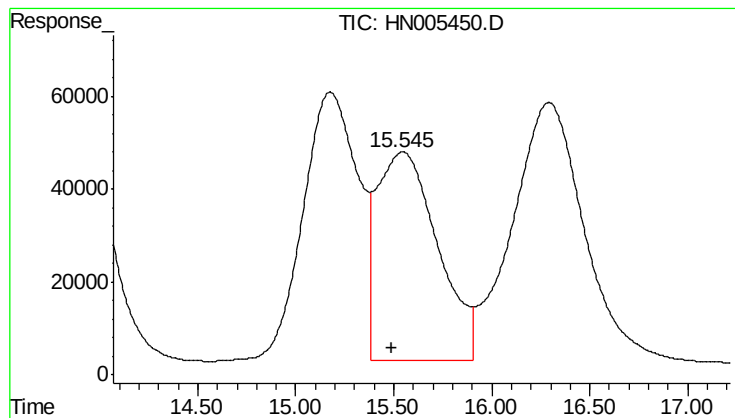

#9 2,4,6-Trinitrotoluene

R.T.: 15.546 min
Delta R.T.: 0.057 min
Response: 9742057
Conc: 392.75 ug/L

Instrument :
HPLC_N
LabSampleId :
HSTDCCC0500