

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN060913\
Data File : HN005455.D
Signal(s) : VWD1A.CH
Acq On : 10-Jun-2013, 02:00
Operator : QM
Sample : HSTDCCC0500
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
HPLC_N
LabSampleId :
HSTDCCC0500

Integration File: autoint1.e
Quant Time: Jun 10 06:54:06 2013
Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN060913.M
Quant Title :
QLast Update : Mon Jun 10 06:49:47 2013
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
5) T 3,5-Dinitroaniline	12.111	9729668	229.588 ng/ml
9) T 2,4,6-Trinitrotoluene	15.550	9036254	364.300 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN060913\
Data File : HN005455.D
Signal(s) : VWD1A.CH
Acq On : 10-Jun-2013, 02:00
Operator : QM
Sample : HSTDCCC0500
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
HPLC_N
LabSampleId :
HSTDCCC0500

Integration File: autoint1.e
Quant Time: Jun 10 06:54:06 2013
Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN060913.M
Quant Title :
QLast Update : Mon Jun 10 06:49:47 2013
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

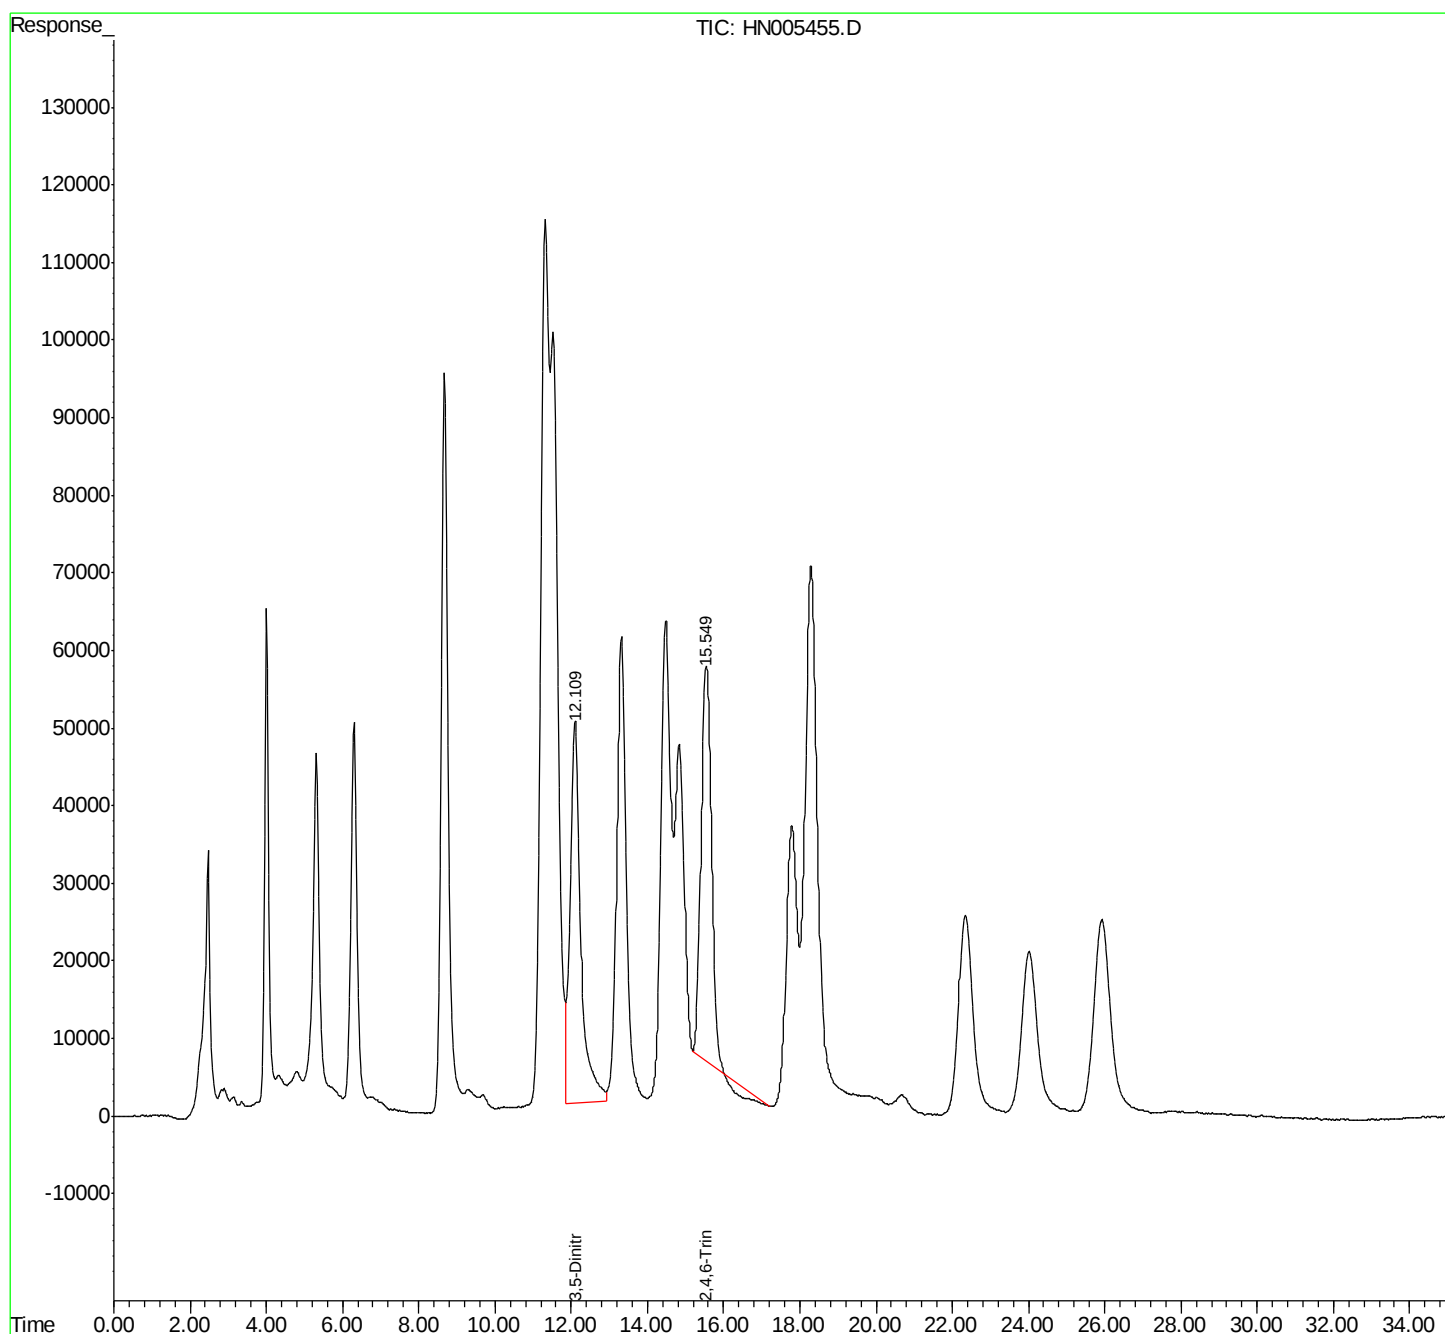


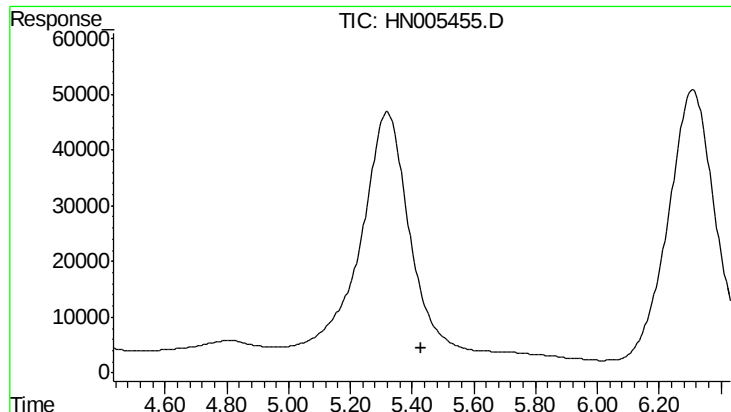

#1 4-Nitroaniline


R.T.: 0.000 min
 Exp R.T.: 5.432 min
 Response: 0
 Conc: N.D.

Instrument :
 HPLC_N
 LabSampleId :
 HSTDCCC0500

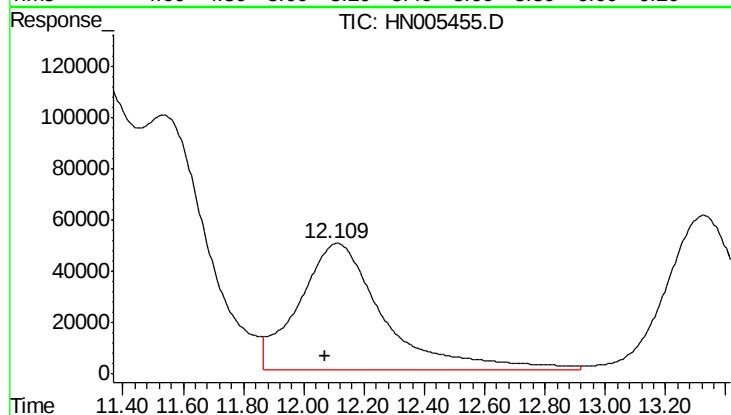

#5 3,5-Dinitroaniline

R.T.: 12.111 min
 Delta R.T.: 0.040 min
 Response: 9729668
 Conc: 229.59 ng/ml

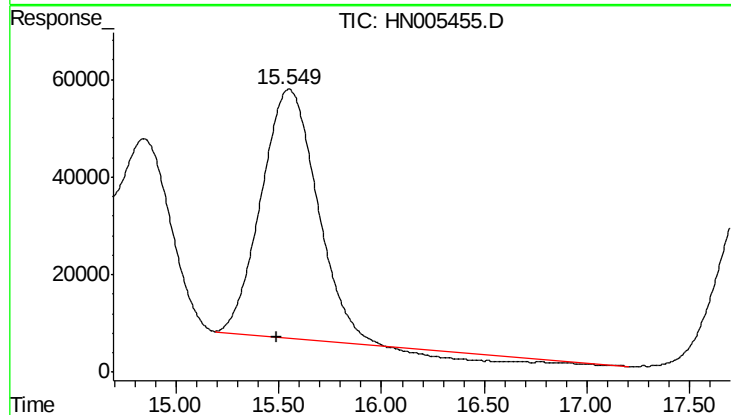

#9 2,4,6-Trinitrotoluene

R.T.: 15.550 min
 Delta R.T.: 0.061 min
 Response: 9036254
 Conc: 364.30 ug/L