

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN062315\
 Data File : HN007394.D
 Signal(s) : vwd1A.ch
 Acq On : 23-Jun-2015, 13:20
 Operator : TP/IZ
 Sample : HSTDICC0200
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 25 02:02:36 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN062315.M
 Quant Title :
 QLast Update : Thu Jun 25 01:35:35 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
1) S	4-Nitroaniline	1.328	897463	239.294 ug/L
Target Compounds				
2) T	HMX	0.891	930142	212.440 ug/L
3) T	RDX	1.705	1288916	231.350 ug/L
4) T	1,3,5-Trinitrobenzene	2.661	2361189	208.464 ug/L
5) T	1,3-Dinitrobenzene	3.528	3547573	193.428 ng/ml
6) T	3,5-Dinitroaniline	3.897	2653919	174.337 ug/L
7) T	Nitrobenzene	4.715	2070058	208.127 ug/L
8) T	Tetryl	6.243	1692277	219.969 ug/L
9) T	2,4,6-Trinitrotoluene	6.504	2387965	208.168 ug/L
10) T	2-Amino-4,6-dinitroto...	7.032	2414804	211.725 ug/L
11) T	4-Amino-2,6-dinitroto...	7.387	2198221	260.467 ug/L
12) T	2,4-Dinitrotoluene	8.120	5143460	275.532 ug/L
13) T	2,6-Dinitrotoluene	8.512	2426205	245.250 ug/L
14) T	2-Nitrotoluene	11.668	1304317	206.391 ug/L
15) T	4-Nitrotoluene	12.418	1143861	212.360 ug/L
16) T	3-Nitrotoluene	13.694	1479125	212.827 ug/L
17) T	PETN	18.789	1815851	185.898 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN062315\
Data File : HN007394.D
Signal(s) : vwd1A.ch
Acq On : 23-Jun-2015, 13:20
Operator : TP/IZ
Sample : HSTDICC0200
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 25 02:02:36 2015
Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN062315.M
Quant Title :
QLast Update : Thu Jun 25 01:35:35 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

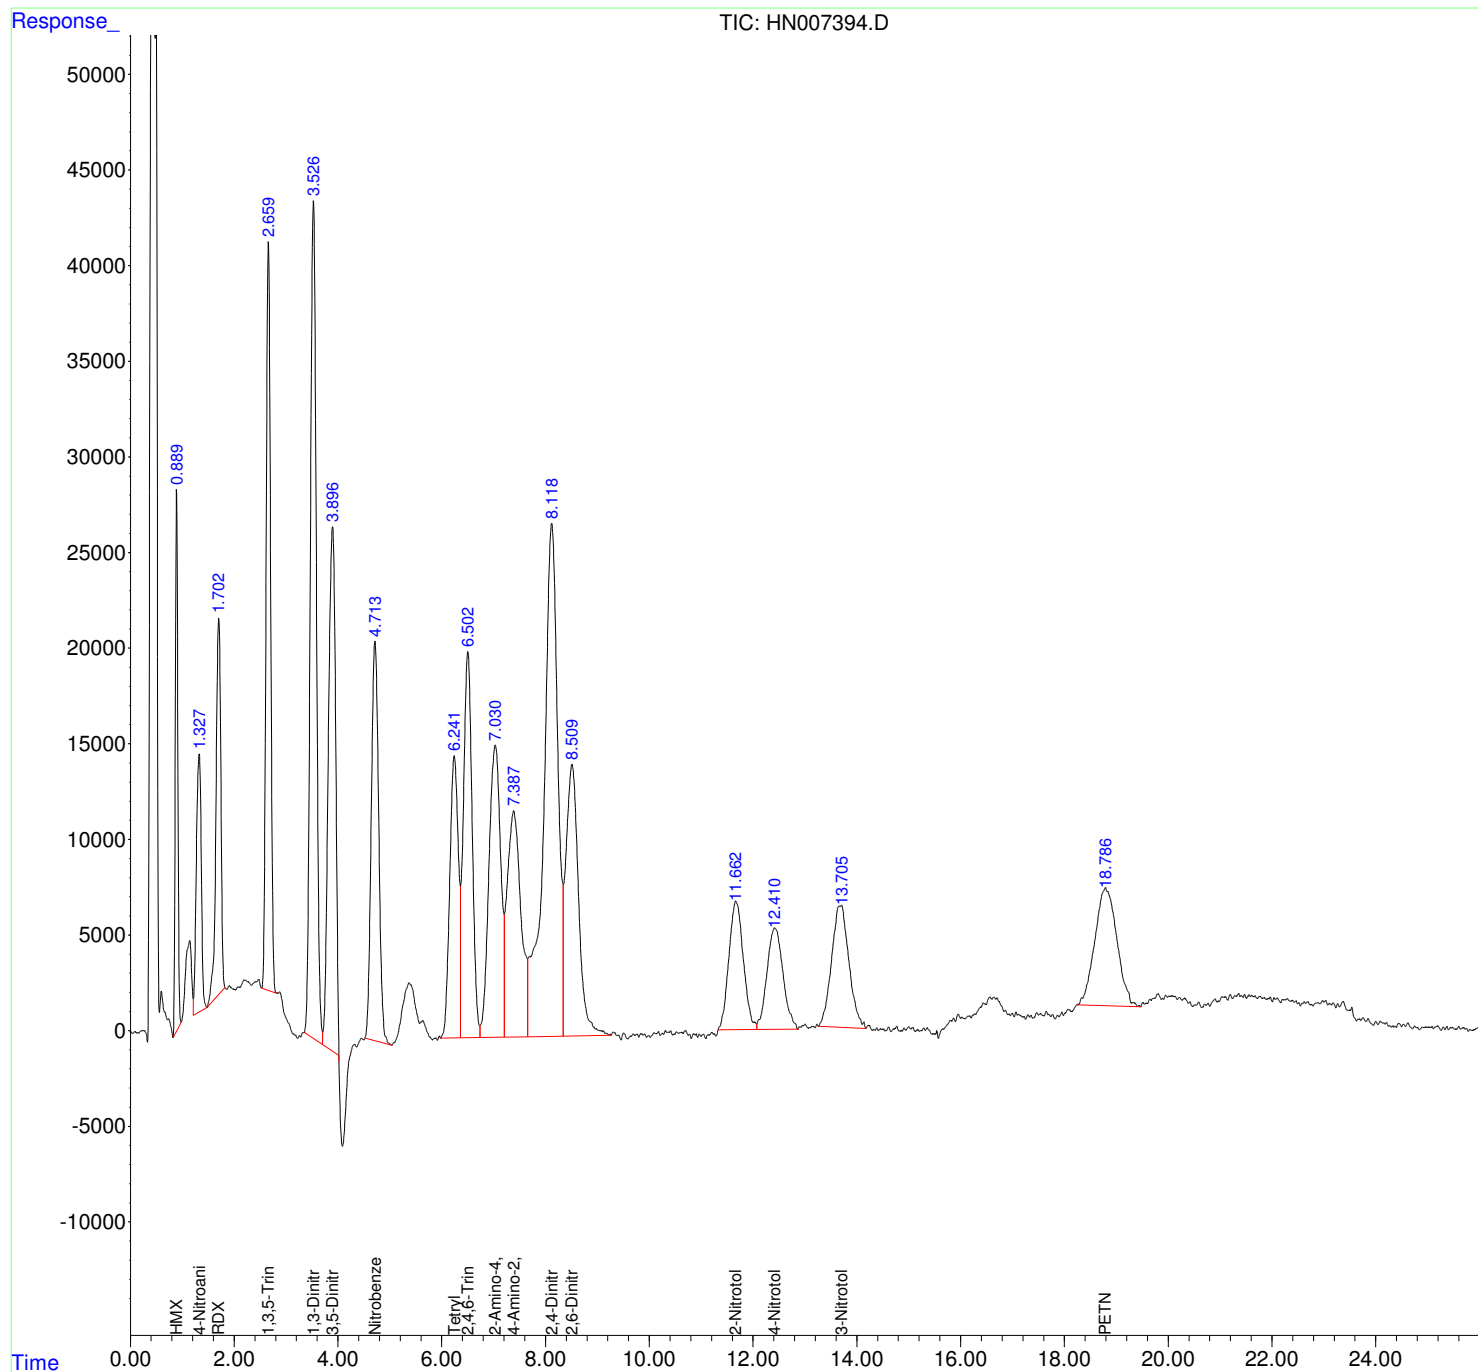


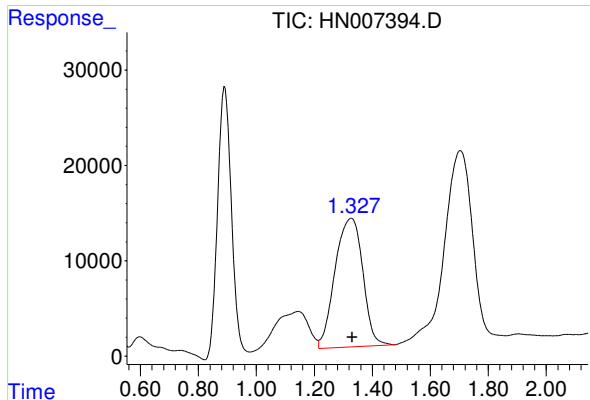

#1 4-Nitroaniline


R.T.: 1.328 min
Delta R.T.: -0.003 min
Response: 897463
Conc: 239.29 ug/L

Instrument :
HPLC_N
ClientSampleId :

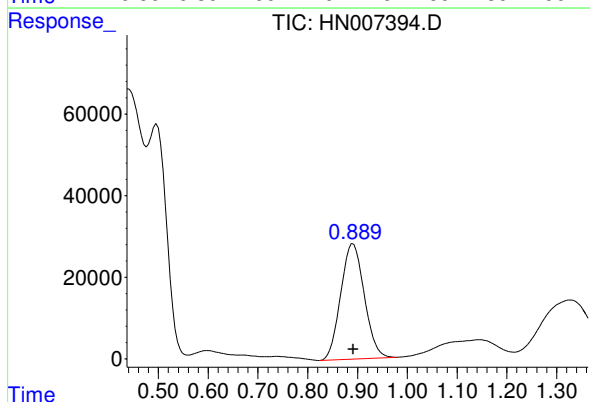


#2 HMX

R.T.: 0.891 min
Delta R.T.: 0.000 min
Response: 930142
Conc: 212.44 ug/L

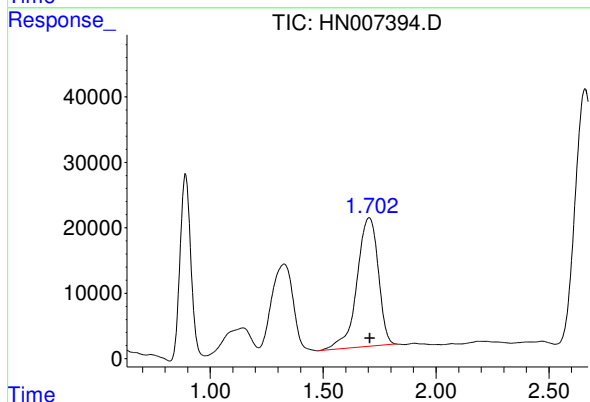


#3 RDX

R.T.: 1.705 min
Delta R.T.: -0.002 min
Response: 1288916
Conc: 231.35 ug/L

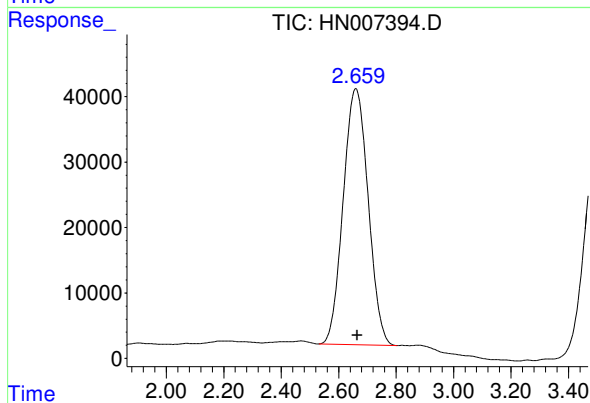

#4 1,3,5-Trinitrobenzene


R.T.: 2.661 min
Delta R.T.: -0.004 min
Response: 2361189
Conc: 208.46 ug/L

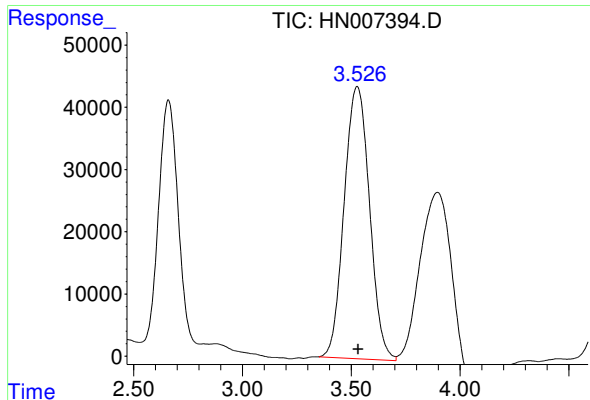

#5 1,3-Dinitrobenzene


R.T.: 3.528 min
Delta R.T.: -0.005 min
Response: 3547573
Conc: 193.43 ng/ml

Instrument :
HPLC_N
ClientSampleId :

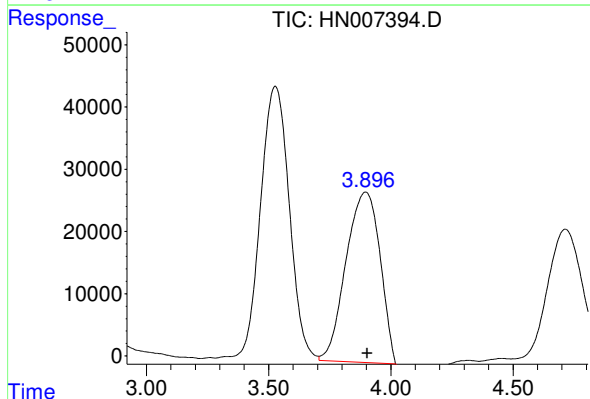


#6 3,5-Dinitroaniline

R.T.: 3.897 min
Delta R.T.: -0.006 min
Response: 2653919
Conc: 174.34 ug/L

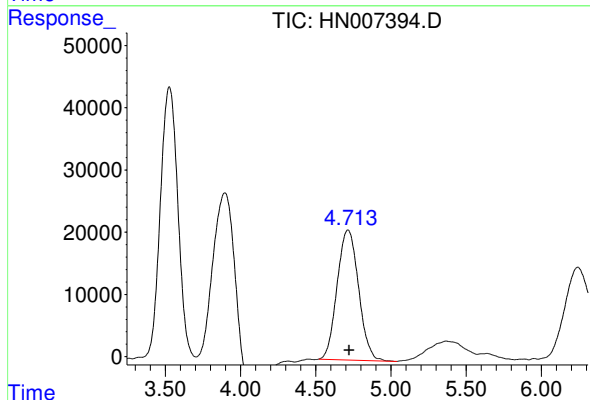


#7 Nitrobenzene

R.T.: 4.715 min
Delta R.T.: -0.008 min
Response: 2070058
Conc: 208.13 ug/L

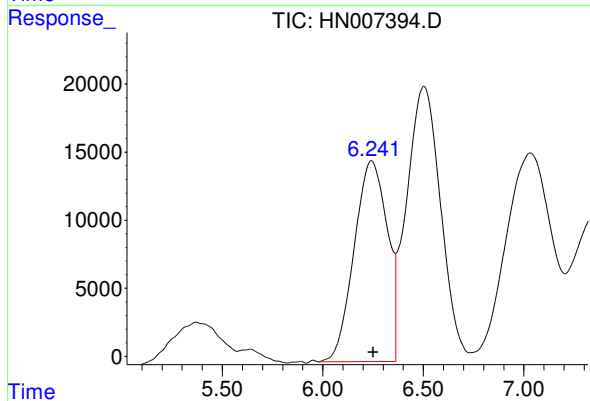

#8 Tetryl


R.T.: 6.243 min
Delta R.T.: -0.009 min
Response: 1692277
Conc: 219.97 ug/L

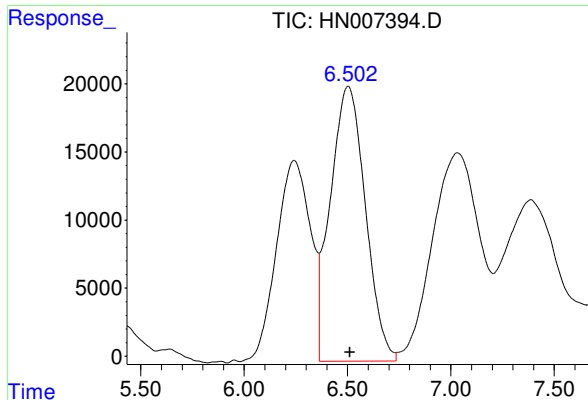

#9 2,4,6-Trinitrotoluene


R.T.: 6.504 min
Delta R.T.: -0.009 min
Response: 2387965
Conc: 208.17 ug/L

Instrument :
HPLC_N
ClientSampleId :

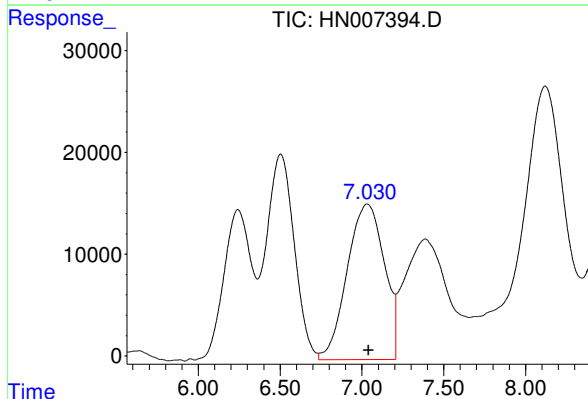


#10 2-Amino-4,6-dinitrotoluene

R.T.: 7.032 min
Delta R.T.: -0.008 min
Response: 2414804
Conc: 211.73 ug/L

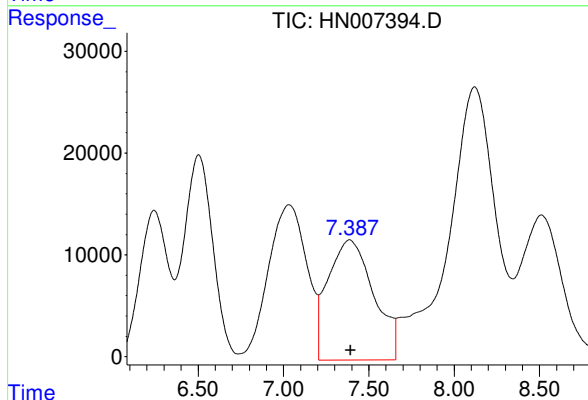


#11 4-Amino-2,6-dinitrotoluene

R.T.: 7.387 min
Delta R.T.: -0.007 min
Response: 2198221
Conc: 260.47 ug/L

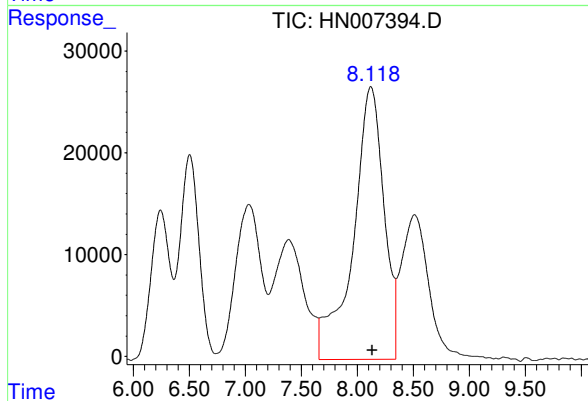

#12 2,4-Dinitrotoluene


R.T.: 8.120 min
Delta R.T.: -0.011 min
Response: 5143460
Conc: 275.53 ug/L

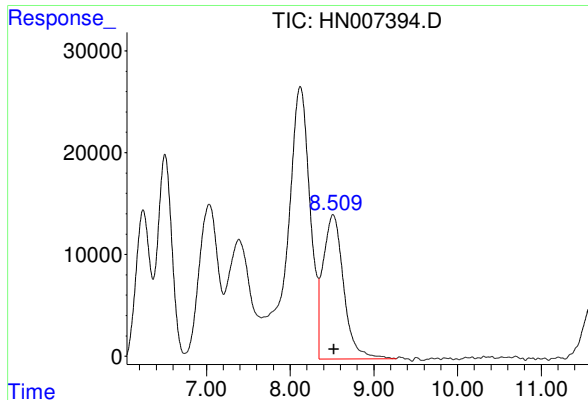

#13 2,6-Dinitrotoluene


R.T.: 8.512 min
Delta R.T.: -0.013 min
Response: 2426205
Conc: 245.25 ug/L

Instrument :
HPLC_N
ClientSampleId :

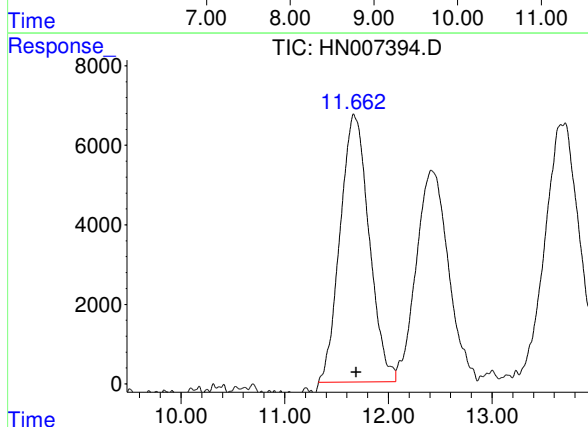


#14 2-Nitrotoluene

R.T.: 11.668 min
Delta R.T.: -0.020 min
Response: 1304317
Conc: 206.39 ug/L

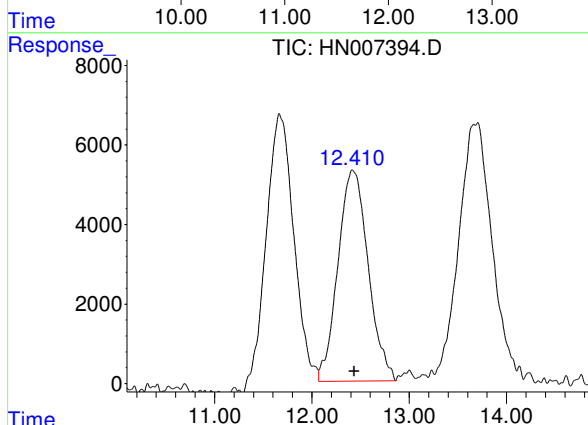


#15 4-Nitrotoluene

R.T.: 12.418 min
Delta R.T.: -0.017 min
Response: 1143861
Conc: 212.36 ug/L

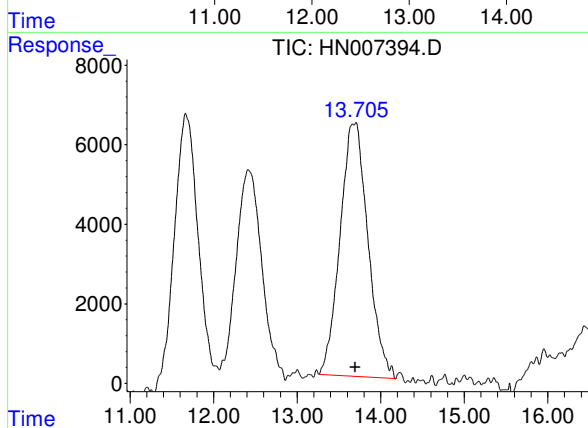

#16 3-Nitrotoluene

R.T.: 13.694 min
Delta R.T.: 0.000 min
Response: 1479125
Conc: 212.83 ug/L

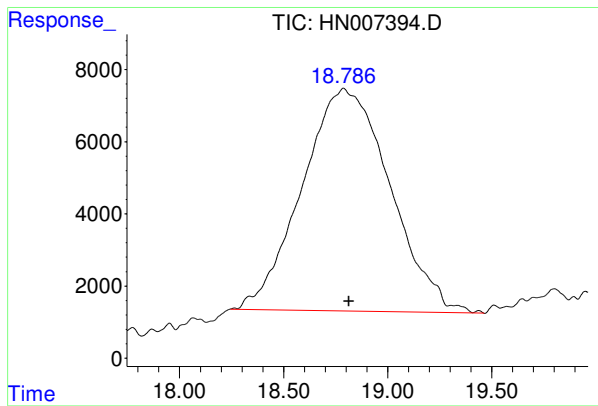

#17 PETN

R.T.: 18.789 min
Delta R.T.: -0.024 min
Response: 1815851
Conc: 185.90 ug/L

Instrument :
HPLC_N
ClientSampleId :