

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN070213\HN005528.D Vial: 6
Acq On : 02-Jul-2013, 13:26 Operator: QM
Sample : HSTDICC0.5 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Jul 2 14:12 2013 Quant Results File: HN070213.RES

Instrument :
HPLC_N
LabSampleId :
HSTDICC0.5

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN070213.M
Title :
Last Update : Tue Jul 02 13:56:28 2013
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.38	2281451	0.551 ng/ul
Target Compounds			
2) T Nitroglycerin	6.35	4412480	0.504 ng/ul

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005528.D HN070213.M

Tue Jul 02 14:12:57 2013

RPT1


Quantitation Report


Data File : Z:\HPCHEM1\HPLC_N\DATA\HN070213\HN005528.D Vial: 6
Acq On : 02-Jul-2013, 13:26 Operator: QM
Sample : HSTDICC0.5 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Jul 2 14:12 2013 Quant Results File: HN070213.RES

Instrument :
HPLC_N
LabSampleId :
HSTDICC0.5

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN070213.M
Title :
Last Update : Tue Jul 02 13:56:28 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

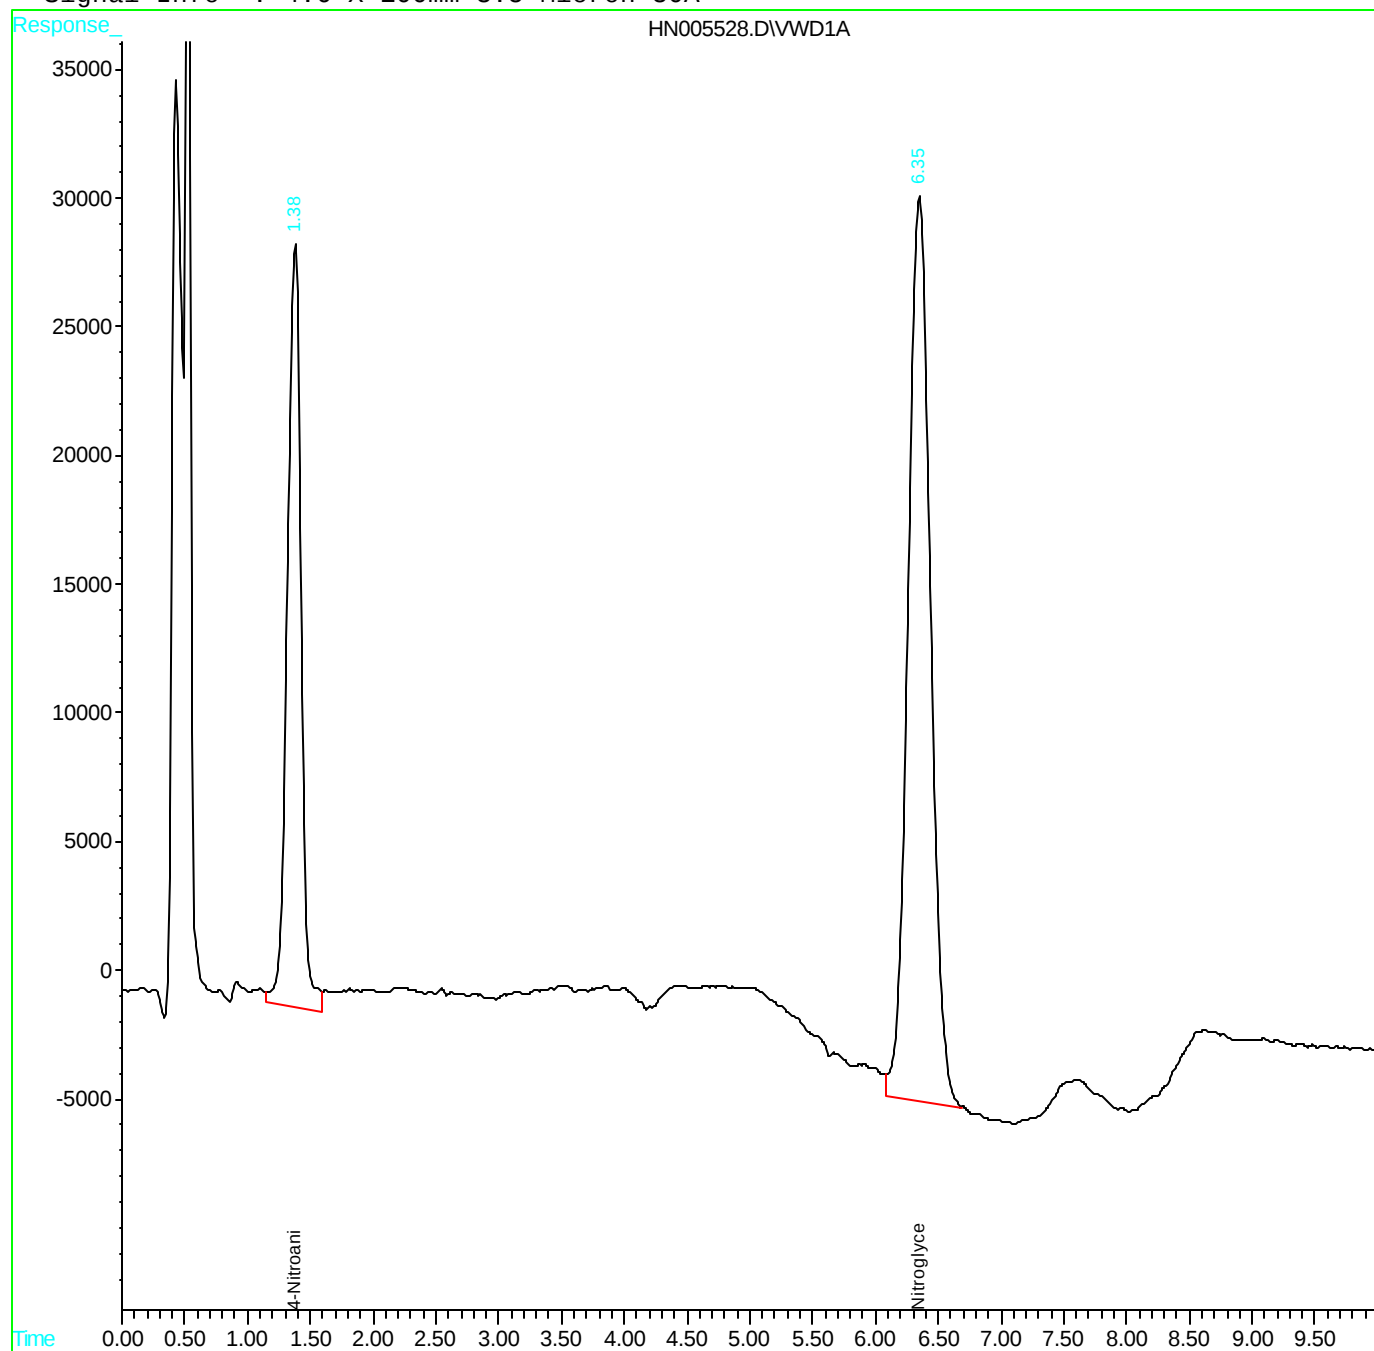


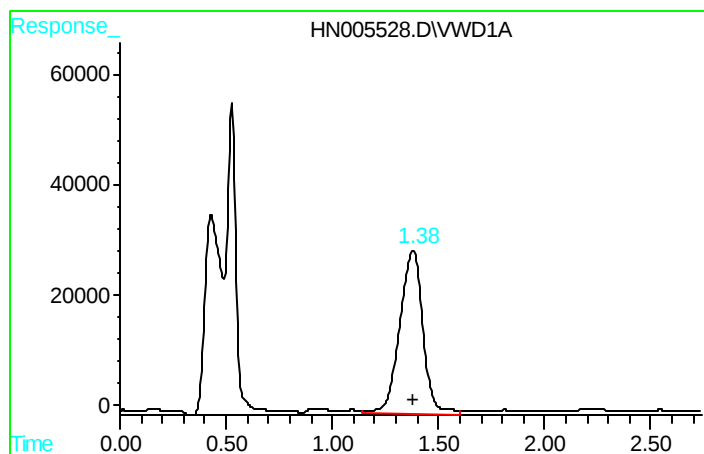

#1 4-Nitroaniline

R.T.: 1.382 min
 Delta R.T.: 0.002 min
 Response: 2281451
 Conc: 0.55 ng/ul

Instrument :
 HPLC_N
 LabSampleId :
 HSTDIC0.5

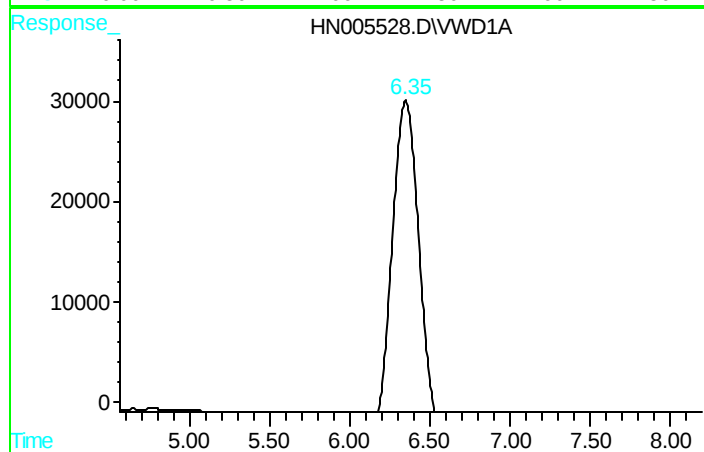

#2 Nitroglycerin

R.T.: 6.350 min
 Delta R.T.: 0.040 min
 Response: 4412480
 Conc: 0.50 ng/ul