

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN070213\HN005523.D Vial: 1
Acq On : 02-Jul-2013, 12:26 Operator: QM
Sample : HSTDICC050 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Jul 2 14:07 2013 Quant Results File: HN070213.RES

Instrument :
HPLC_N
LabSampleId :
HSTDICC050

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN070213.M
Title :
Last Update : Tue Jul 02 13:56:28 2013
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.38	206001833	49.722 ng/ul
Target Compounds			
2) T Nitroglycerin	6.31	429067647	48.968 ng/ul

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005523.D HN070213.M

Tue Jul 02 14:18:09 2013

RPT1


Quantitation Report


Data File : Z:\HPCHEM1\HPLC_N\DATA\HN070213\HN005523.D Vial: 1
Acq On : 02-Jul-2013, 12:26 Operator: QM
Sample : HSTDICC050 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Jul 2 14:07 2013 Quant Results File: HN070213.RES

Instrument :
HPLC_N
LabSampleId :
HSTDICC050

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN070213.M
Title :
Last Update : Tue Jul 02 13:56:28 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

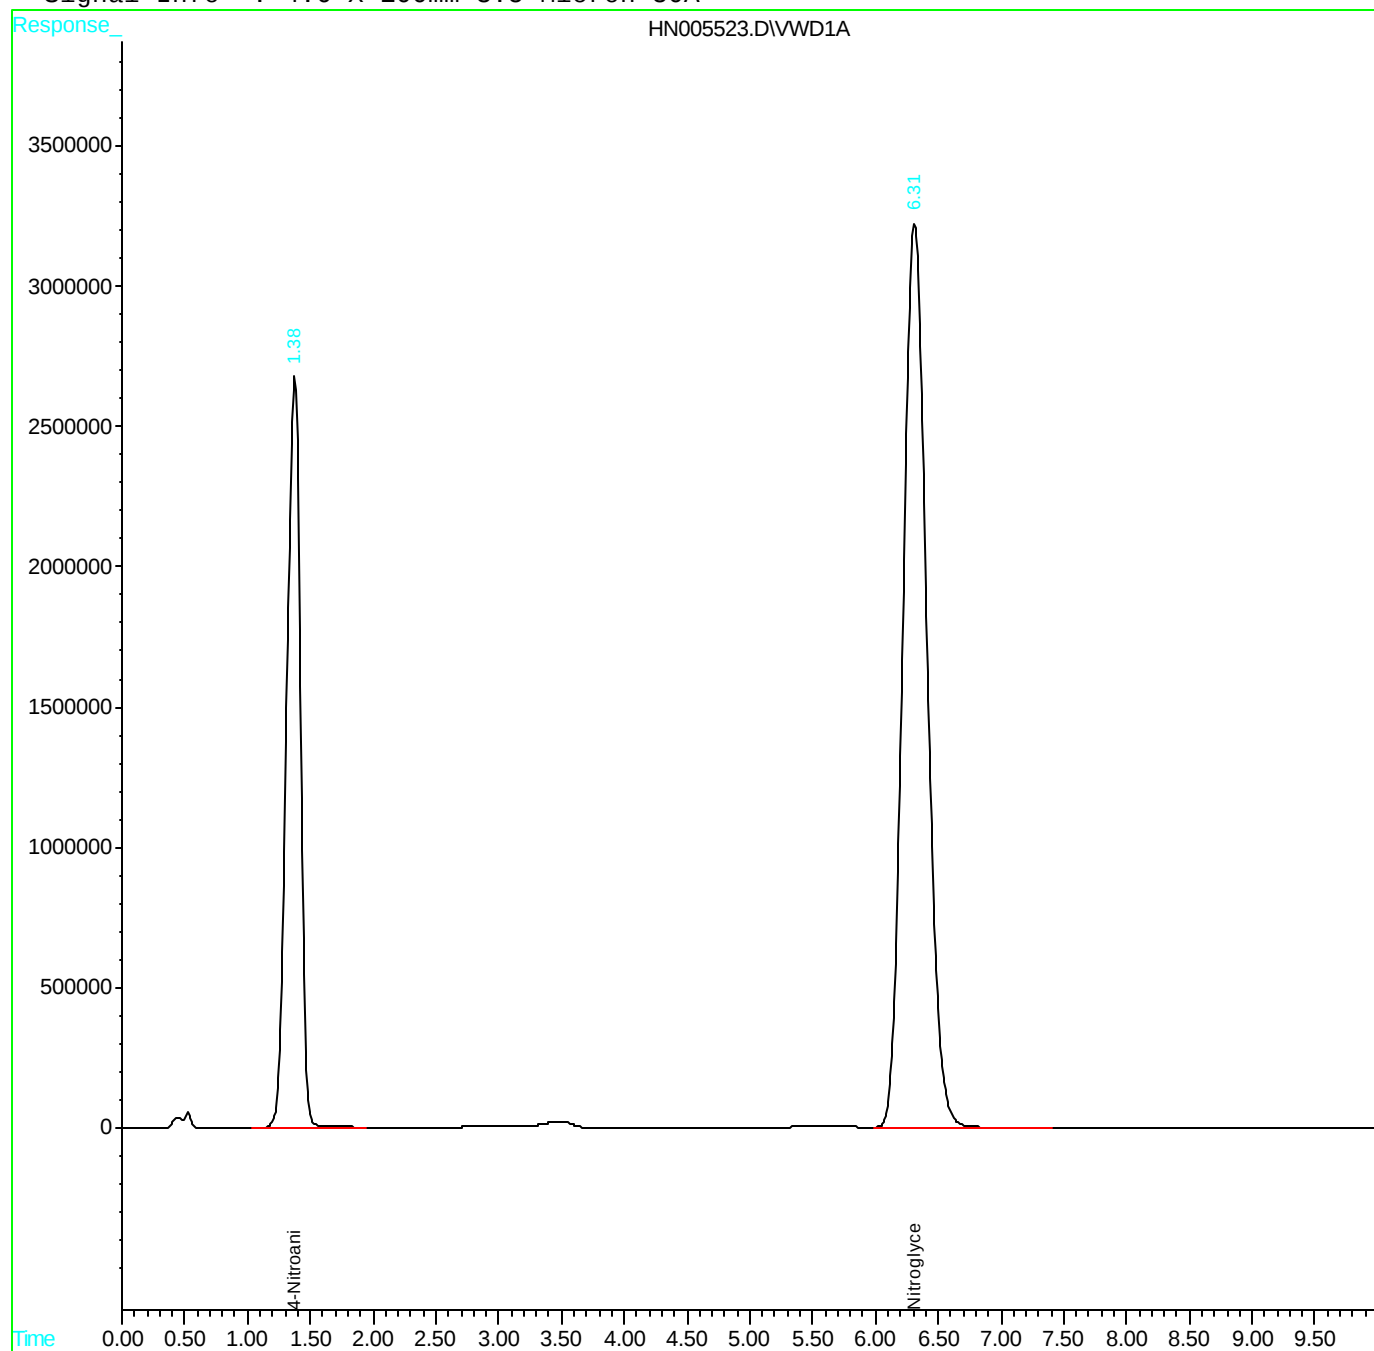


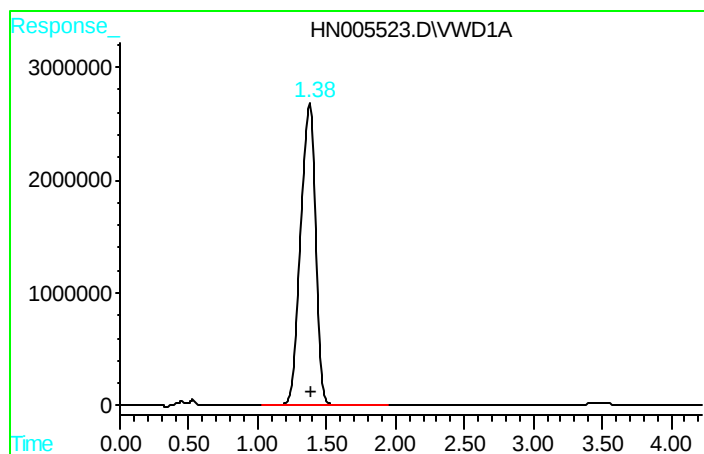

#1 4-Nitroaniline

R.T.: 1.379 min
 Delta R.T.: 0.000 min
 Response: 206001833
 Conc: 49.72 ng/ul

Instrument :
 HPLC_N
 LabSampleId :
 HSTDIC050

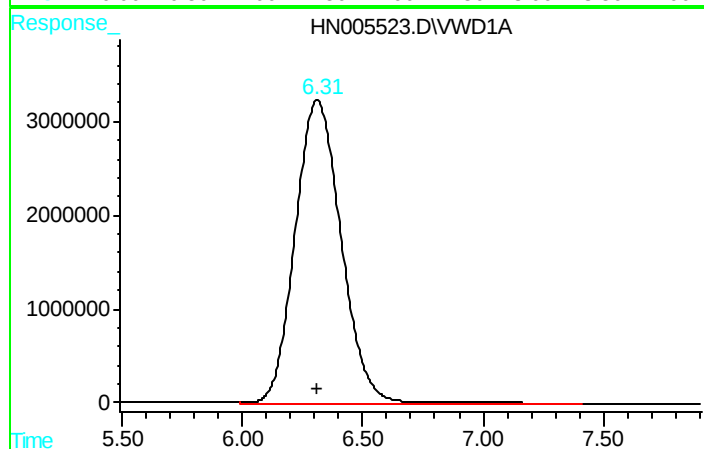

#2 Nitroglycerin

R.T.: 6.312 min
 Delta R.T.: 0.002 min
 Response: 429067647
 Conc: 48.97 ng/ul