

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN070213\HN005525.D Vial: 3
Acq On : 02-Jul-2013, 12:50 Operator: QM
Sample : HSTDICC010 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Jul 2 14:09 2013 Quant Results File: HN070213.RES

Instrument :
HPLC_N
LabSampleId :
HSTDICC010

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN070213.M
Title :
Last Update : Tue Jul 02 13:56:28 2013
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.39	42301116	10.210 ng/ul
Target Compounds			
2) T Nitroglycerin	6.34	87829228	10.024 ng/ul

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005525.D HN070213.M

Tue Jul 02 14:18:43 2013

RPT1


Quantitation Report


Data File : Z:\HPCHEM1\HPLC_N\DATA\HN070213\HN005525.D Vial: 3
Acq On : 02-Jul-2013, 12:50 Operator: QM
Sample : HSTDICC010 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Jul 2 14:09 2013 Quant Results File: HN070213.RES

Instrument :
HPLC_N
LabSampleId :
HSTDICC010

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN070213.M
Title :
Last Update : Tue Jul 02 13:56:28 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

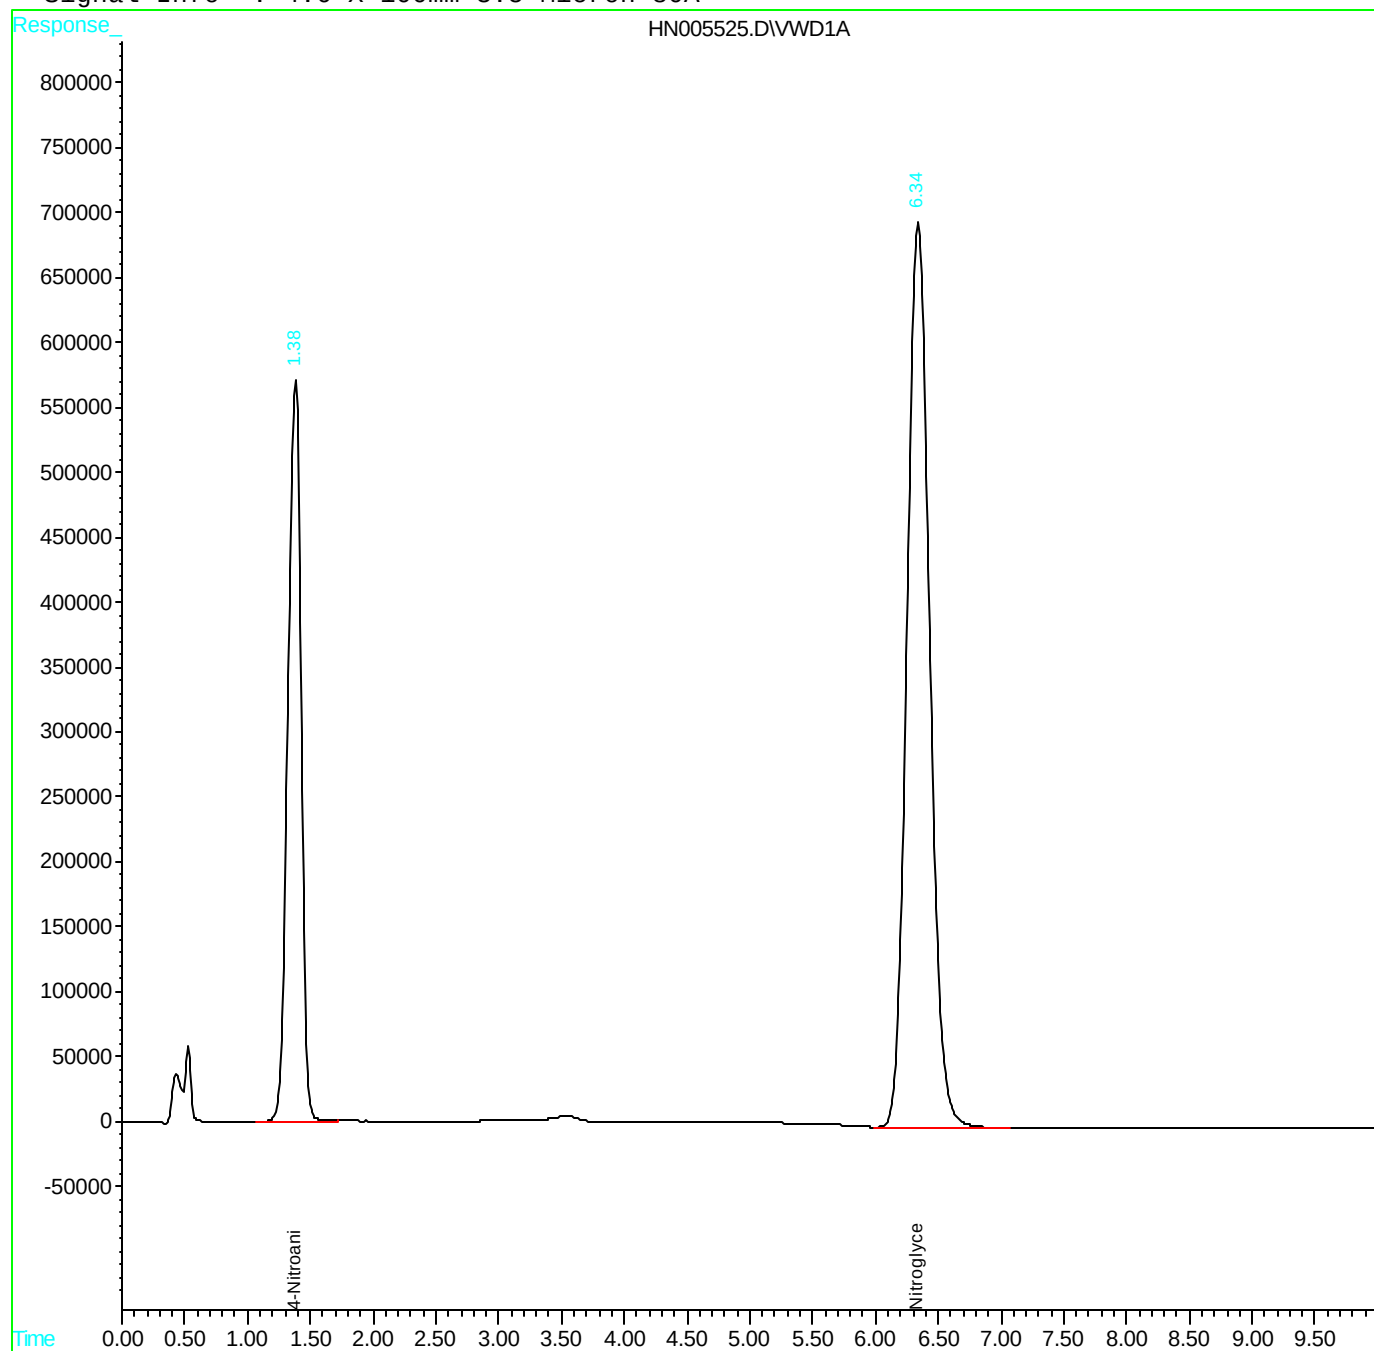


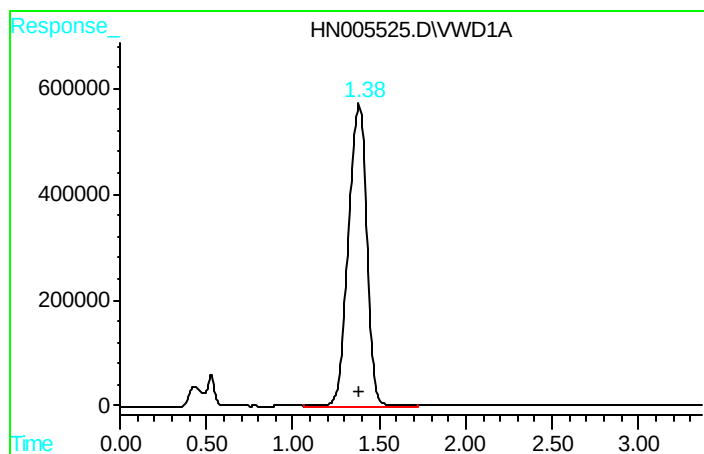

#1 4-Nitroaniline

R.T.: 1.385 min
Delta R.T.: 0.005 min
Response: 42301116
Conc: 10.21 ng/ul

Instrument :
HPLC_N
LabSampleId :
HSTDIC010

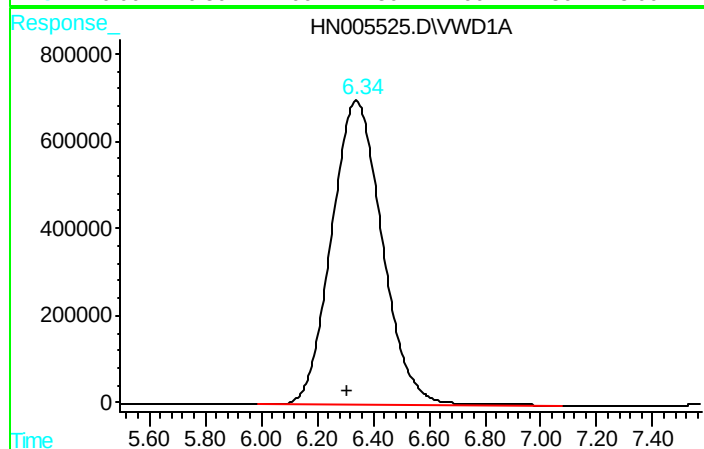

#2 Nitroglycerin

R.T.: 6.341 min
Delta R.T.: 0.031 min
Response: 87829228
Conc: 10.02 ng/ul