

Data File : Z:\HPCHEM1\HPLC\_N\DATA\HN070213\HN005529.D Vial: 7  
Acq On : 02-Jul-2013, 13:38 Operator: QM  
Sample : HSTDICV005 Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : AUTOINT1.E  
Quant Time: Jul 2 14:16 2013 Quant Results File: HN070213.RES

Instrument :  
HPLC\_N  
ClientSampleId :  
ICVHN070213

Quant Method : Z:\HPCHEM1\HPLC\_N\METHOD\HN070213.M  
Title :  
Last Update : Tue Jul 02 14:14:07 2013  
Response via : Initial Calibration  
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

| Compound                    | R.T. | Response | Conc Units  |
|-----------------------------|------|----------|-------------|
| -----                       |      |          |             |
| System Monitoring Compounds |      |          |             |
| 1) S 4-Nitroaniline         | 1.39 | 22719357 | 5.345 ng/ul |
| Target Compounds            |      |          |             |
| 2) T Nitroglycerin          | 6.30 | 41785621 | 4.782 ng/ul |

-----  
Analyst Signature:\_\_\_\_\_ Analyst Name:\_\_\_\_\_ Date:\_\_\_\_\_

-----REASONS FOR MANUAL INTEGRATIONS-----

\_\_\_Poor resolution of peaks exhibited on chromatogram.Compound #:\_\_\_\_\_

\_\_\_Peak Integrated by software incorrectly.Compound #:\_\_\_\_\_

\_\_\_OTHER:\_\_\_\_\_Compound #:\_\_\_\_\_

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005529.D HN070213.M

Tue Jul 02 14:17:50 2013

RPT1


# Quantitation Report


Data File : Z:\HPCHEM1\HPLC\_N\DATA\HN070213\HN005529.D Vial: 7  
Acq On : 02-Jul-2013, 13:38 Operator: QM  
Sample : HSTDICV005 Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : AUTOINT1.E  
Quant Time: Jul 2 14:16 2013 Quant Results File: HN070213.RES

Instrument :  
HPLC\_N  
ClientSampleId :  
ICVHN070213

Quant Method : Z:\HPCHEM1\HPLC\_N\METHOD\HN070213.M  
Title :  
Last Update : Tue Jul 02 14:14:07 2013  
Response via : Multiple Level Calibration  
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

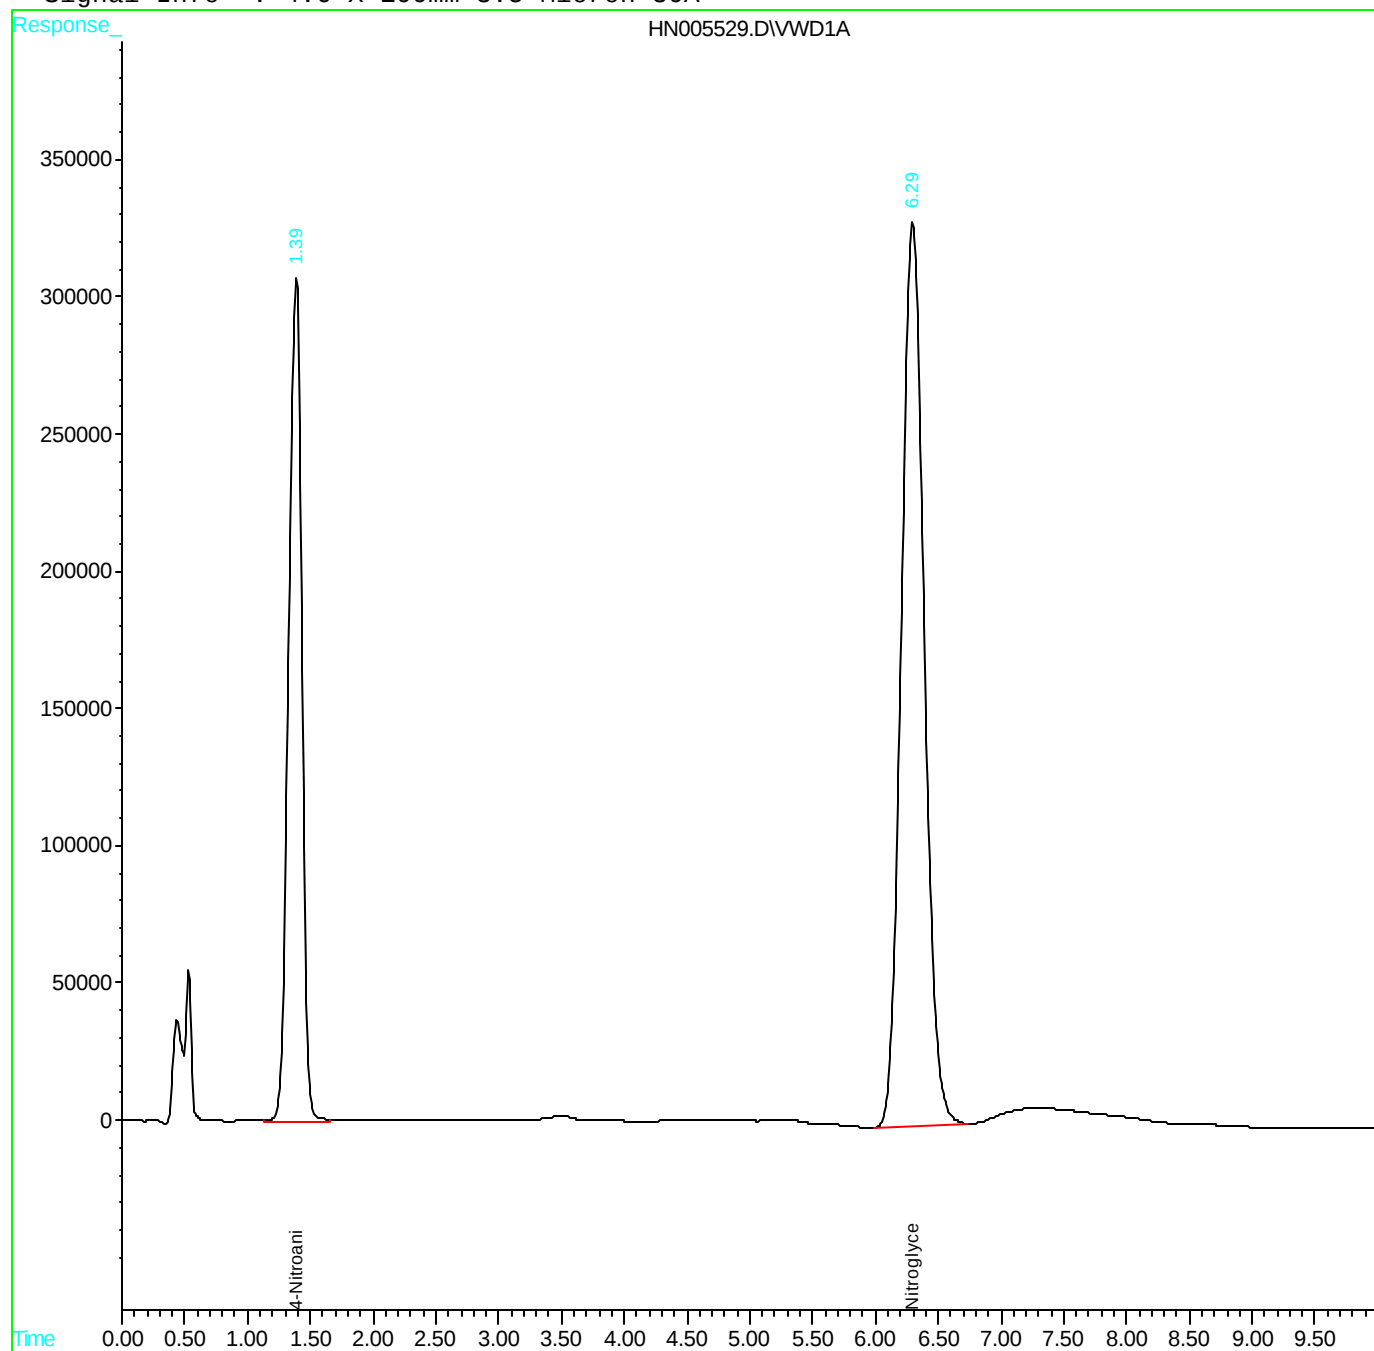


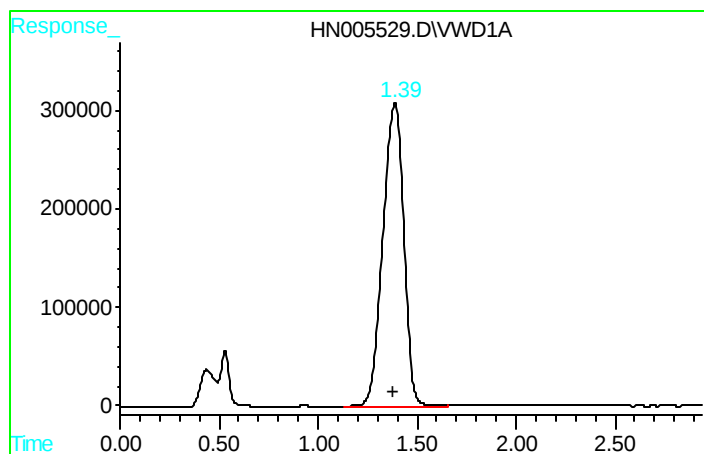

#1 4-Nitroaniline

R.T.: 1.391 min  
 Delta R.T.: 0.011 min  
 Response: 22719357  
 Conc: 5.35 ng/ul

Instrument :  
 HPLC\_N  
 ClientSampleId :  
 ICVHN070213

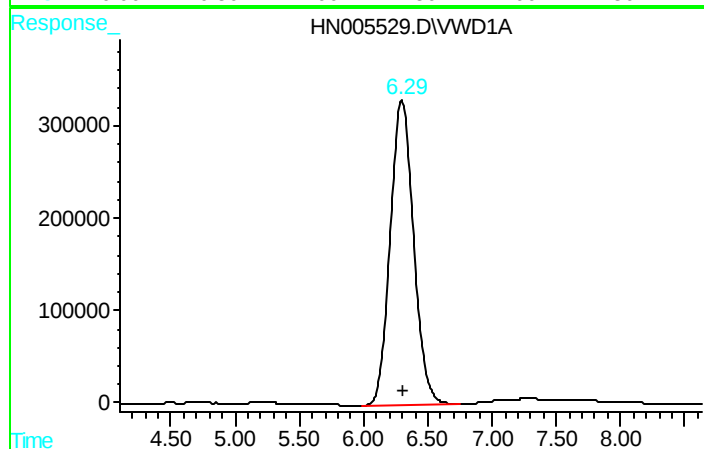

#2 Nitroglycerin

R.T.: 6.297 min  
 Delta R.T.: -0.013 min  
 Response: 41785621  
 Conc: 4.78 ng/ul