

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN070313\HN005562.D Vial: 7
Acq On : 03-Jul-2013, 16:43 Operator: QM
Sample : E2748-16MS Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Jul 5 10:04 2013 Quant Results File: HN070213.RES

Instrument :
HPLC_N
ClientSampleId :
POLJAT01-SB-DUP-062713MS

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN070213.M
Title :
Last Update : Fri Jul 05 10:04:06 2013
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.38	770003	0.181 ng/ul
Target Compounds			
2) T Nitroglycerin	6.32	1315450	0.151 ng/ul

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005562.D HN070213.M

Fri Jul 05 10:04:11 2013

RPT1


Quantitation Report


Data File : Z:\HPCHEM1\HPLC_N\DATA\HN070313\HN005562.D Vial: 7
Acq On : 03-Jul-2013, 16:43 Operator: QM
Sample : E2748-16MS Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Jul 5 10:04 2013 Quant Results File: HN070213.RES

Instrument :
HPLC_N
ClientSampleId :
POLJAT01-SB-DUP-062713MS

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN070213.M
Title :
Last Update : Fri Jul 05 10:04:06 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

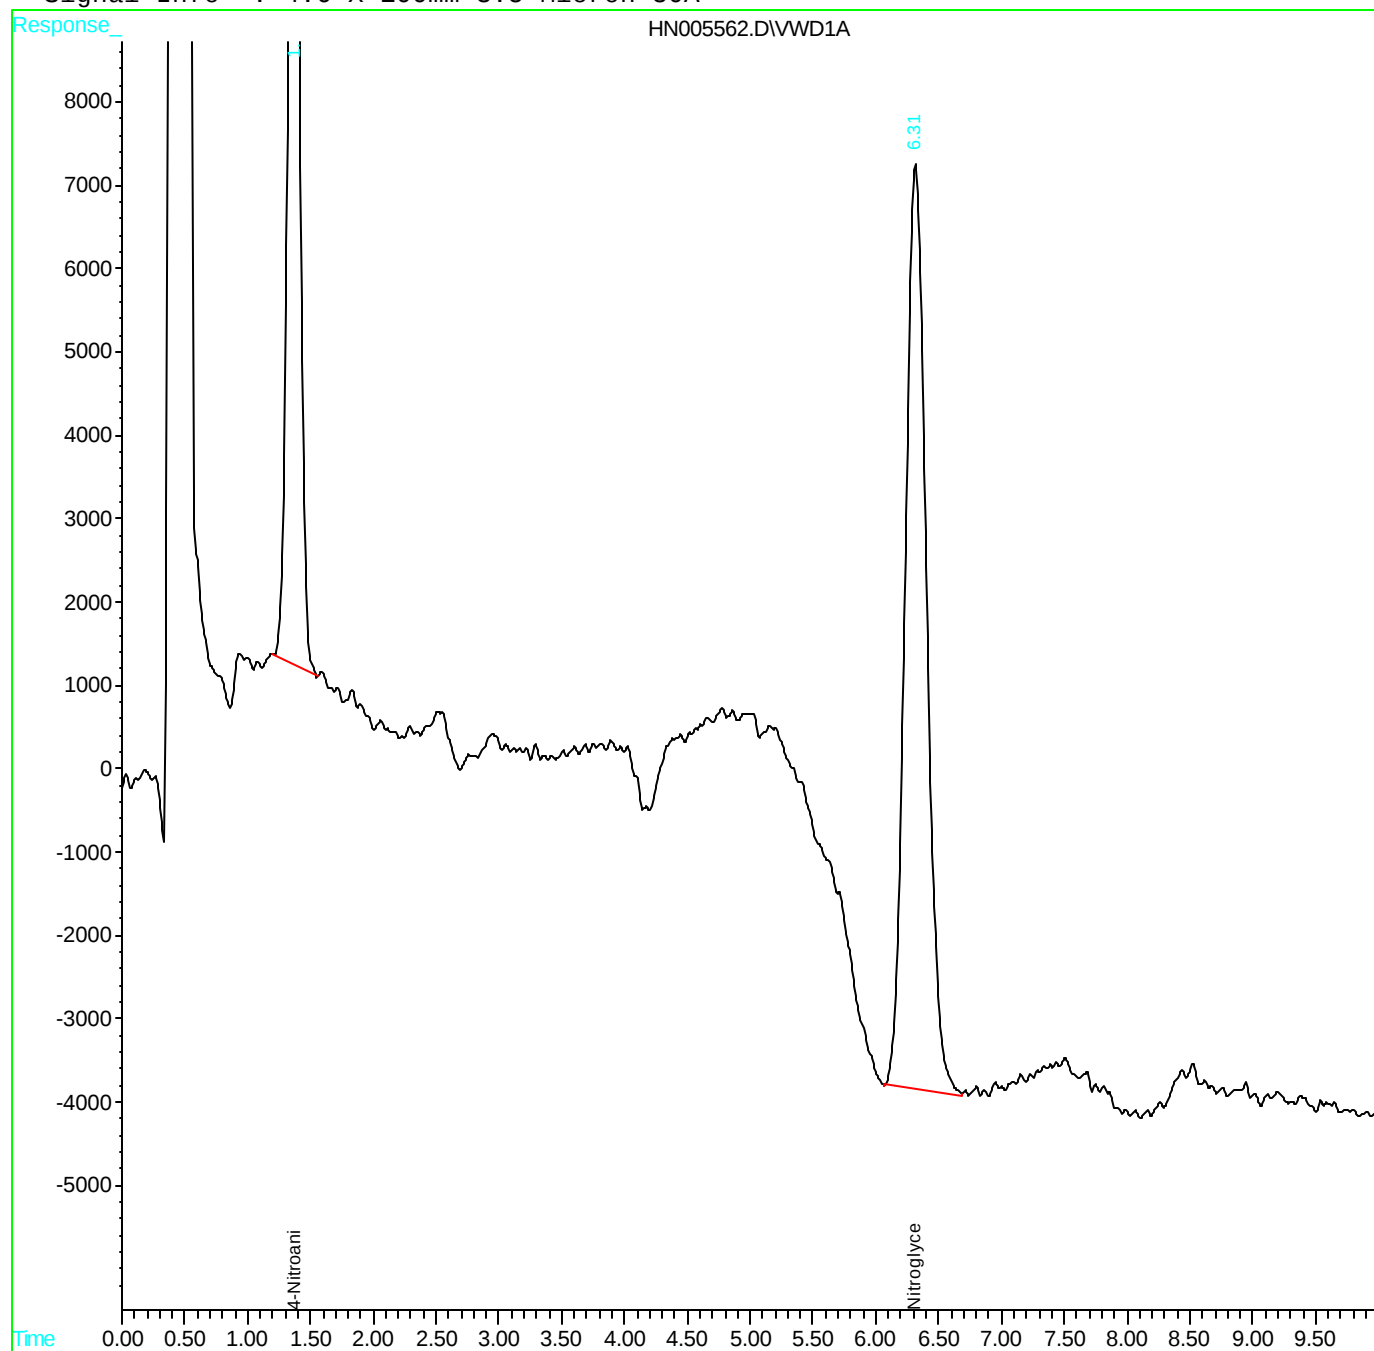


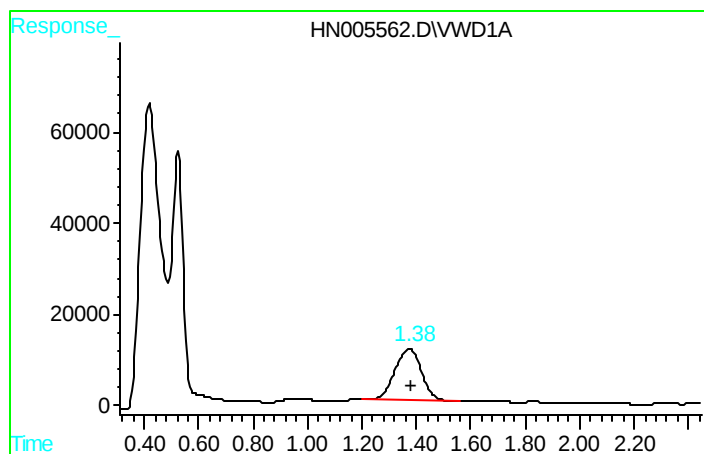

#1 4-Nitroaniline

R.T.: 1.378 min
 Delta R.T.: -0.002 min
 Response: 770003
 Conc: 0.18 ng/ul

Instrument :
 HPLC_N
 ClientSampleId :
 POLJAT01-SB-DUP-062713MS

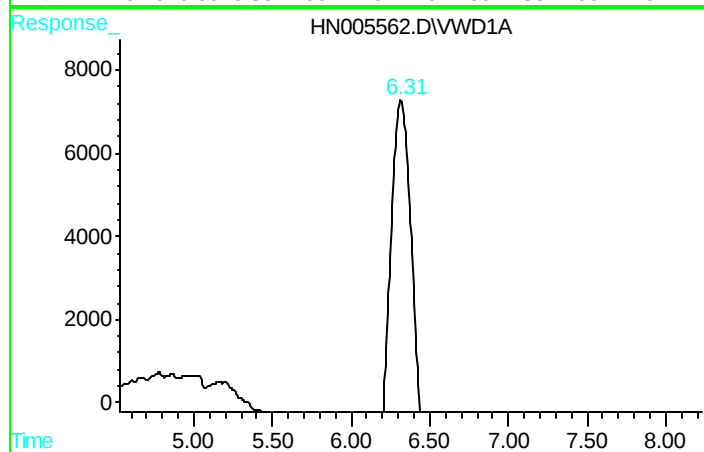

#2 Nitroglycerin

R.T.: 6.317 min
 Delta R.T.: -0.003 min
 Response: 1315450
 Conc: 0.15 ng/ul