

Data File : Z:\HPCHEM1\HPLC\_N\DATA\HN070313\HN005564.D Vial: 9  
Acq On : 03-Jul-2013, 17:07 Operator: QM  
Sample : E2748-16 Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : AUTOINT1.E  
Quant Time: Jul 5 10:05 2013 Quant Results File: HN070213.RES

Instrument :  
HPLC\_N  
ClientSampleId :  
POLJAT01-SB-DUP-062713

Quant Method : Z:\HPCHEM1\HPLC\_N\METHOD\HN070213.M  
Title :  
Last Update : Fri Jul 05 10:04:06 2013  
Response via : Initial Calibration  
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

| Compound                    | R.T. | Response | Conc Units  |
|-----------------------------|------|----------|-------------|
| -----                       |      |          |             |
| System Monitoring Compounds |      |          |             |
| 1) S 4-Nitroaniline         | 1.39 | 711659   | 0.167 ng/ul |
| Target Compounds            |      |          |             |
| 2) T Nitroglycerin          | 6.30 | 293344   | 0.034 ng/ul |

-----  
Analyst Signature:\_\_\_\_\_ Analyst Name:\_\_\_\_\_ Date:\_\_\_\_\_

-----REASONS FOR MANUAL INTEGRATIONS-----

\_\_\_Poor resolution of peaks exhibited on chromatogram.Compound #:\_\_\_\_\_

\_\_\_Peak Integrated by software incorrectly.Compound #:\_\_\_\_\_

\_\_\_OTHER:\_\_\_\_\_Compound #:\_\_\_\_\_

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005564.D HN070213.M

Fri Jul 05 10:05:01 2013

RPT1


# Quantitation Report


Data File : Z:\HPCHEM1\HPLC\_N\DATA\HN070313\HN005564.D Vial: 9  
Acq On : 03-Jul-2013, 17:07 Operator: QM  
Sample : E2748-16 Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : AUTOINT1.E  
Quant Time: Jul 5 10:05 2013 Quant Results File: HN070213.RES

Instrument :  
HPLC\_N  
ClientSampleId :  
POLJAT01-SB-DUP-062713

Quant Method : Z:\HPCHEM1\HPLC\_N\METHOD\HN070213.M  
Title :  
Last Update : Fri Jul 05 10:04:06 2013  
Response via : Multiple Level Calibration  
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

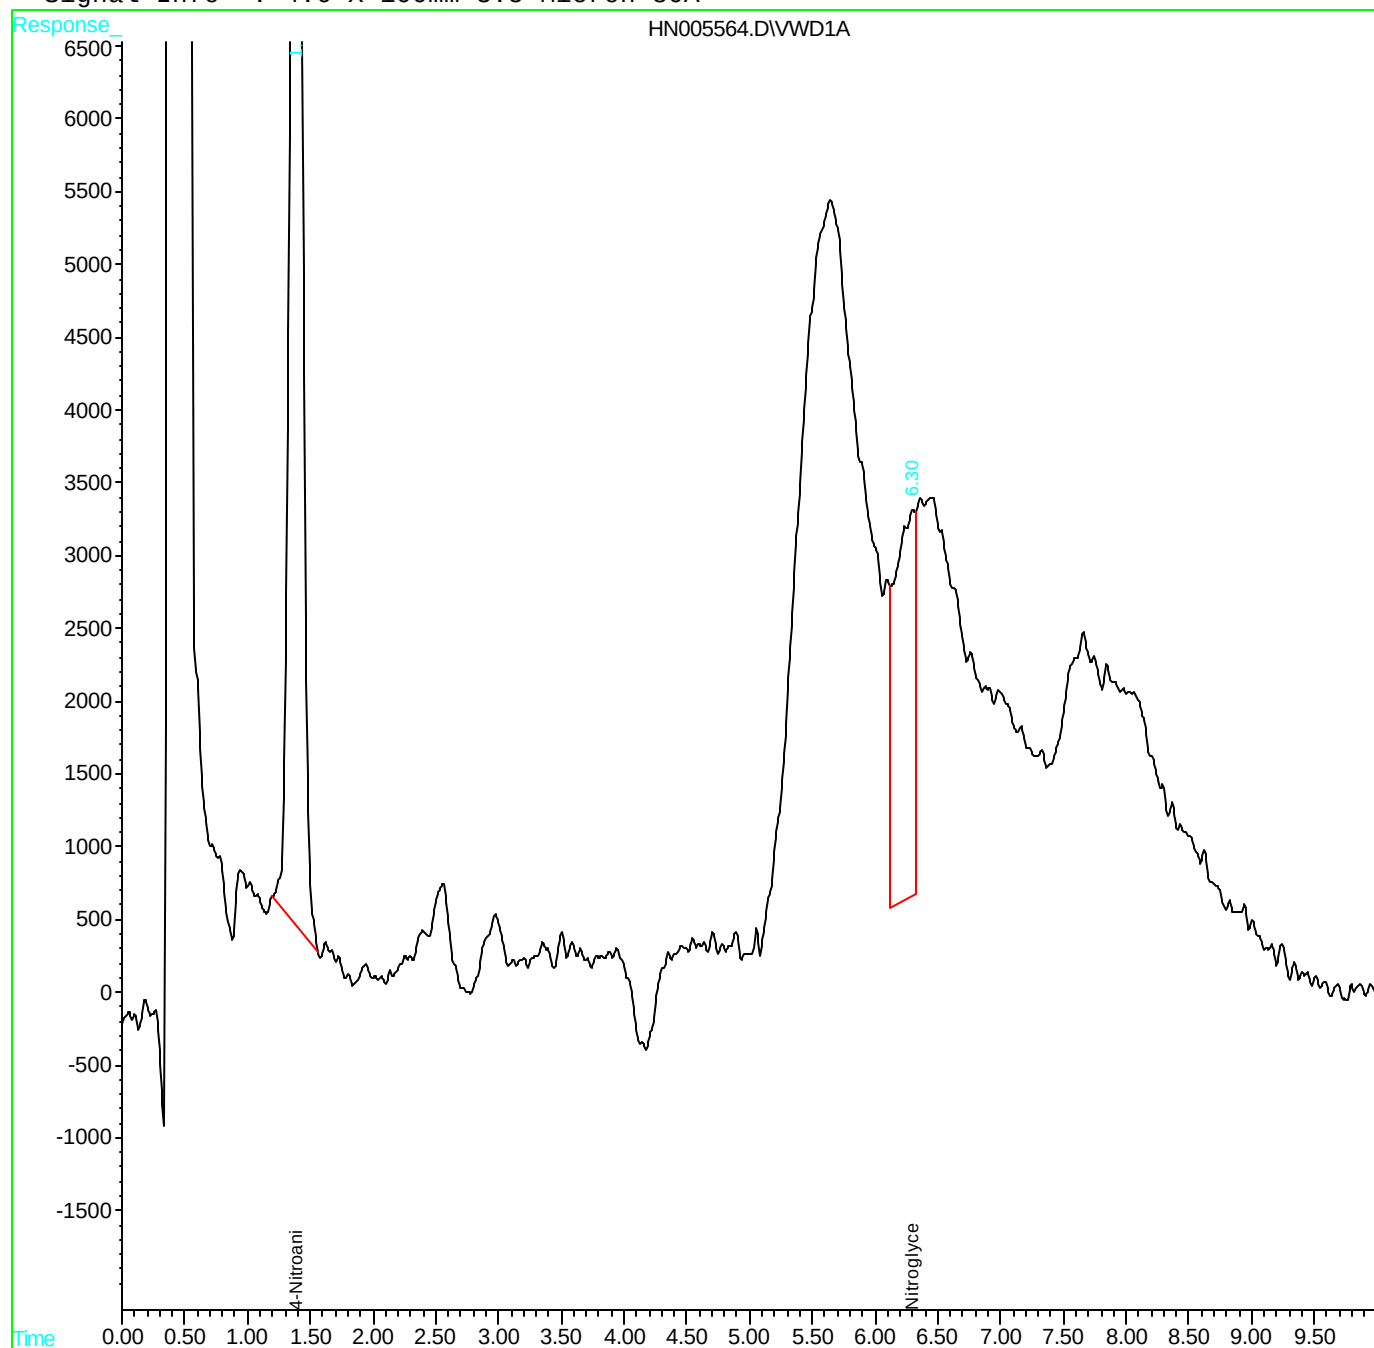


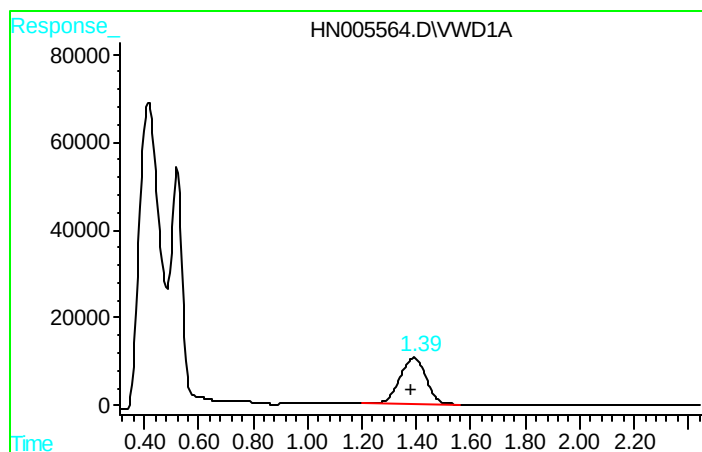

# #1 4-Nitroaniline

R.T.: 1.394 min  
Delta R.T.: 0.014 min  
Response: 711659  
Conc: 0.17 ng/ul

Instrument :  
HPLC\_N  
ClientSampleId :  
POLJAT01-SB-DUP-062713

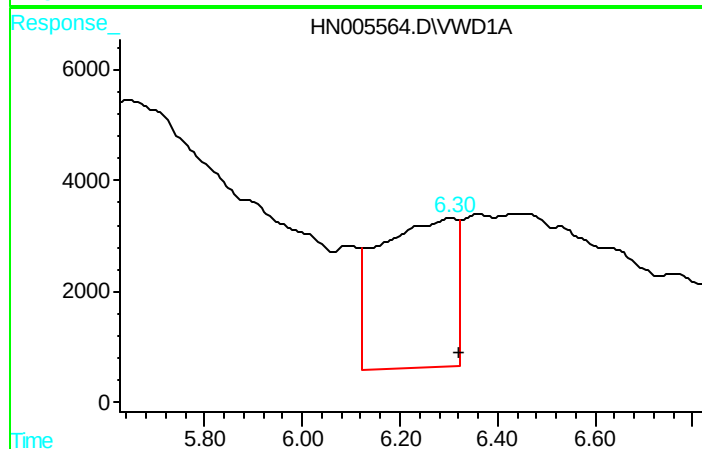

# #2 Nitroglycerin

R.T.: 6.303 min  
Delta R.T.: -0.017 min  
Response: 293344  
Conc: 0.03 ng/ul