

Data File : S:\HPCHEM1\HPLC_N\DATA\HN070913\HN005587.D Vial: 47
Acq On : 09-Jul-2013, 11:33 Operator: QM
Sample : E2797-02 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Jul 9 15:54 2013 Quant Results File: HN070213.RES

Instrument :
HPLC_N
ClientSampleId :
B537-MW-2

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN070213.M
Title :
Last Update : Tue Jul 09 09:58:42 2013
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.35	1226042	0.288 ng/ul

Target Compounds

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005587.D HN070213.M

Thu Jul 11 06:26:05 2013

RPT1


Quantitation Report


Data File : S:\HPCHEM1\HPLC_N\DATA\HN070913\HN005587.D Vial: 47
Acq On : 09-Jul-2013, 11:33 Operator: QM
Sample : E2797-02 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Jul 9 15:54 2013 Quant Results File: HN070213.RES

Instrument :
HPLC_N
ClientSampleId :
B537-MW-2

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN070213.M
Title :
Last Update : Tue Jul 09 09:58:42 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

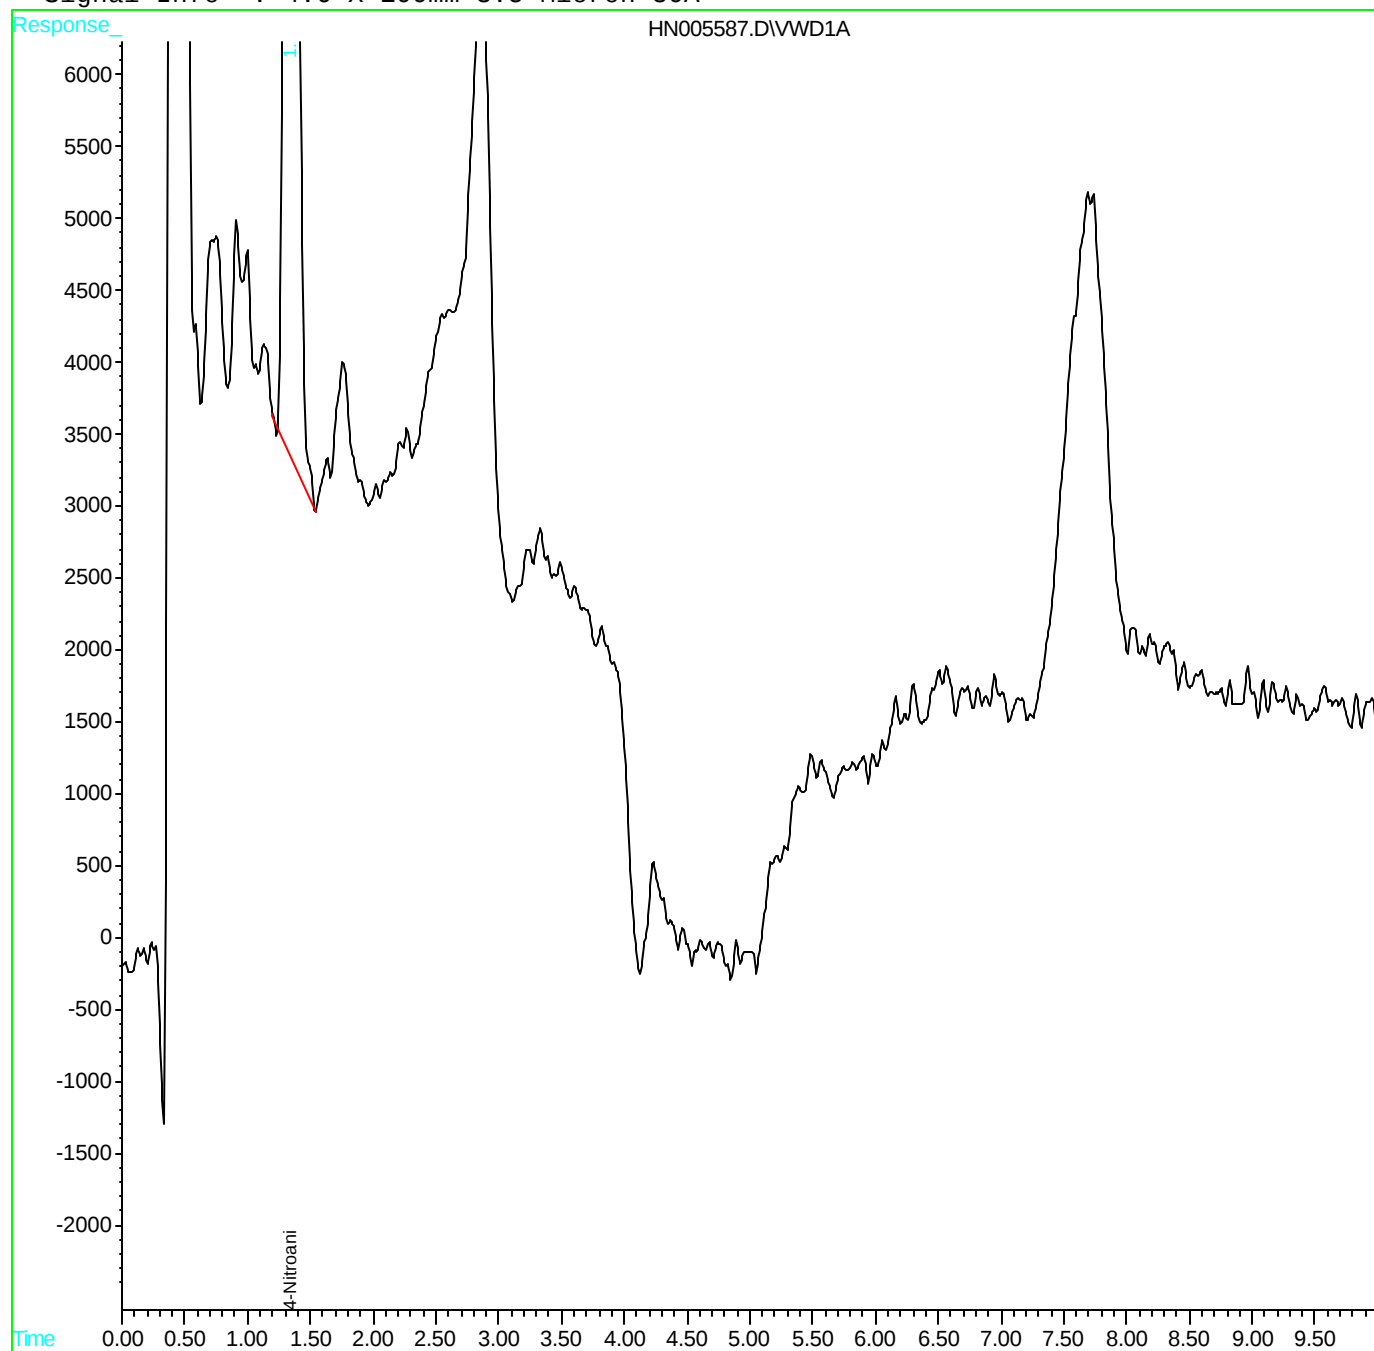

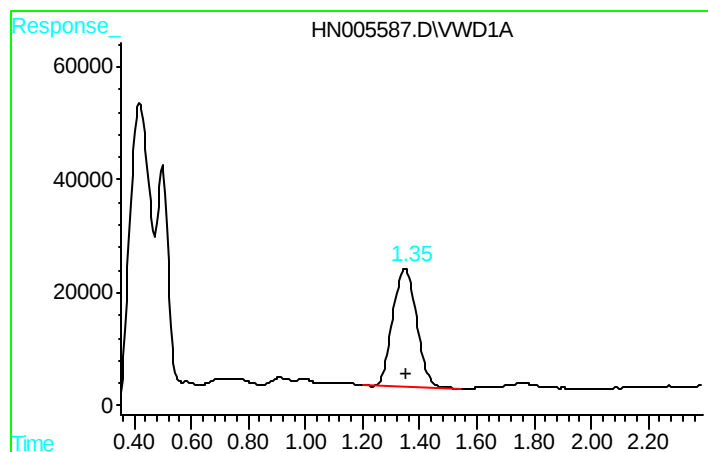

#1 4-Nitroaniline

R.T.: 1.350 min
Delta R.T.: 0.000 min
Response: 1226042
Conc: 0.29 ng/ul

Instrument :
HPLC_N
ClientSampleId :
B537-MW-2