

Data File : S:\HPCHEM1\HPLC_N\DATA\HN071113\HN005598.D Vial: 1
Acq On : 11-Jul-2013, 16:18 Operator: QM
Sample : HSTDCCC005 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Jul 11 14:04 2013 Quant Results File: HN070213.RES

Instrument :
HPLC_N
LabSampleId :
HSTDCCC005

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN070213.M
Title :
Last Update : Tue Jul 02 14:14:07 2013
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005598.D HN070213.M

Fri Jul 12 10:15:22 2013

RPT1


Quantitation Report


Data File : S:\HPCHEM1\HPLC_N\DATA\HN071113\HN005598.D Vial: 1
Acq On : 11-Jul-2013, 16:18 Operator: QM
Sample : HSTDCCC005 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Jul 11 14:04 2013 Quant Results File: HN070213.RES

Instrument :
HPLC_N
LabSampleId :
HSTDCCC005

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN070213.M
Title :
Last Update : Tue Jul 02 14:14:07 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

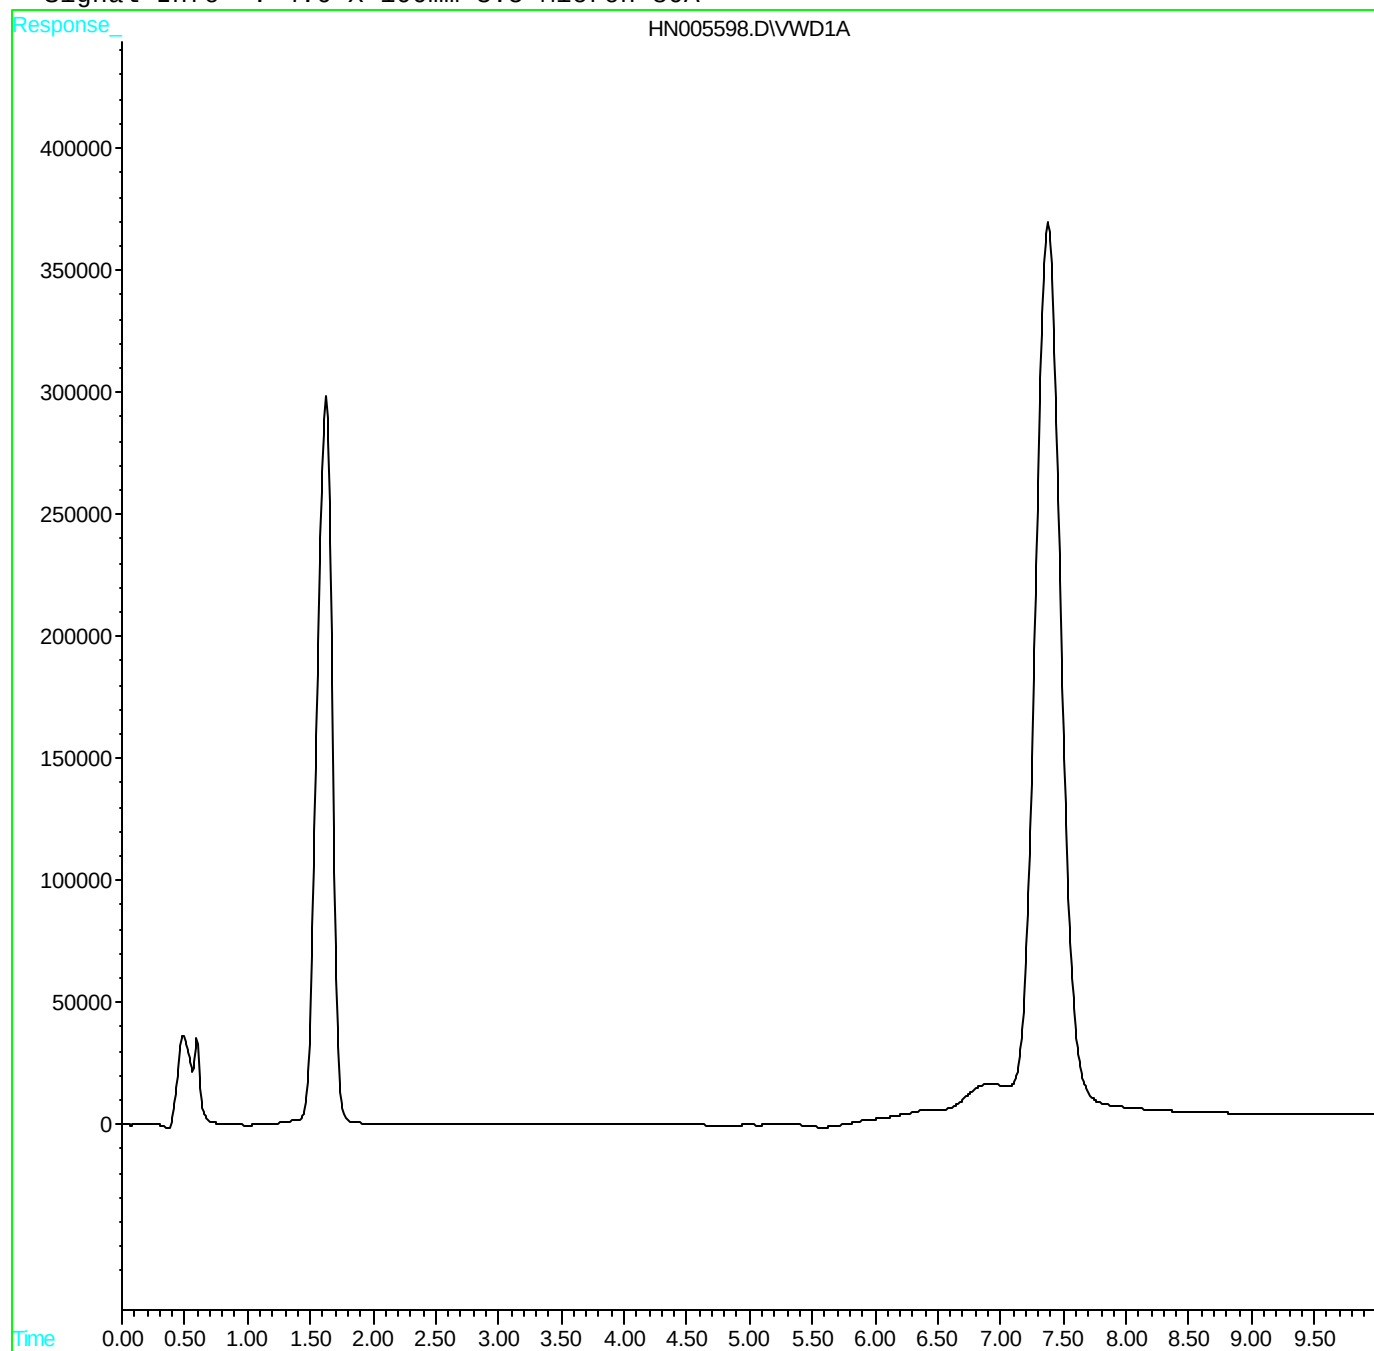

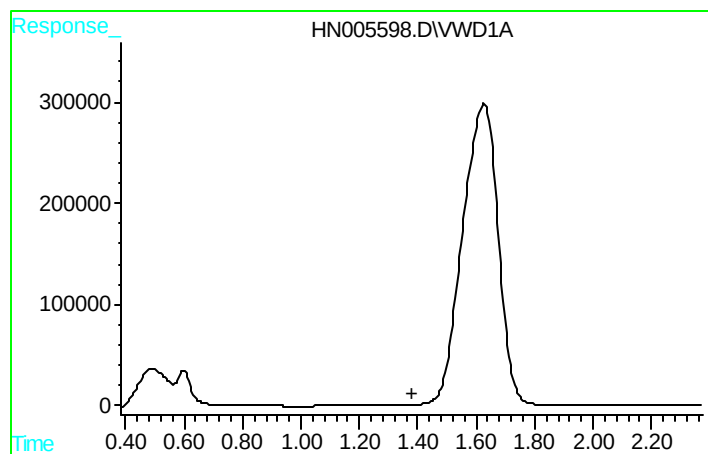

#1 4-Nitroaniline

R.T.: 0.000 min
Exp R.T. : 1.380 min
Response: 0
Conc: N.D.

Instrument :
HPLC_N
LabSampleId :
HSTDCCC005