

Data File : S:\HPCHEM1\HPLC\_N\DATA\HN071113\HN005615.D Vial: 19  
Acq On : 11-Jul-2013, 20:43 Operator: QM  
Sample : E2837-01MS Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : AUTOINT1.E  
Quant Time: Jul 12 8:36 2013 Quant Results File: HN071113.RES

Instrument :  
HPLC\_N  
ClientSampleId :  
BG500SS01AMS

Quant Method : Z:\HPCHEM1\HPLC\_N\METHOD\HN071113.M  
Title :  
Last Update : Fri Jul 12 08:34:40 2013  
Response via : Initial Calibration  
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

| Compound                    | R.T. | Response | Conc Units  |
|-----------------------------|------|----------|-------------|
| -----                       |      |          |             |
| System Monitoring Compounds |      |          |             |
| 1) S 4-Nitroaniline         | 1.40 | 725025   | 0.168 ng/ul |
| Target Compounds            |      |          |             |
| 2) T Nitroglycerin          | 6.40 | 1191387  | 0.128 ng/ul |

-----  
Analyst Signature:\_\_\_\_\_ Analyst Name:\_\_\_\_\_ Date:\_\_\_\_\_

-----REASONS FOR MANUAL INTEGRATIONS-----

\_\_\_Poor resolution of peaks exhibited on chromatogram.Compound #:\_\_\_\_\_

\_\_\_Peak Integrated by software incorrectly.Compound #:\_\_\_\_\_

\_\_\_OTHER:\_\_\_\_\_Compound #:\_\_\_\_\_

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005615.D HN071113.M Fri Jul 12 08:36:21 2013 RPT1


# Quantitation Report


Data File : S:\HPCHEM1\HPLC\_N\DATA\HN071113\HN005615.D Vial: 19  
Acq On : 11-Jul-2013, 20:43 Operator: QM  
Sample : E2837-01MS Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : AUTOINT1.E  
Quant Time: Jul 12 8:36 2013 Quant Results File: HN071113.RES

Instrument :  
HPLC\_N  
ClientSampleId :  
BG500SS01AMS

Quant Method : Z:\HPCHEM1\HPLC\_N\METHOD\HN071113.M  
Title :  
Last Update : Fri Jul 12 08:34:40 2013  
Response via : Multiple Level Calibration  
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

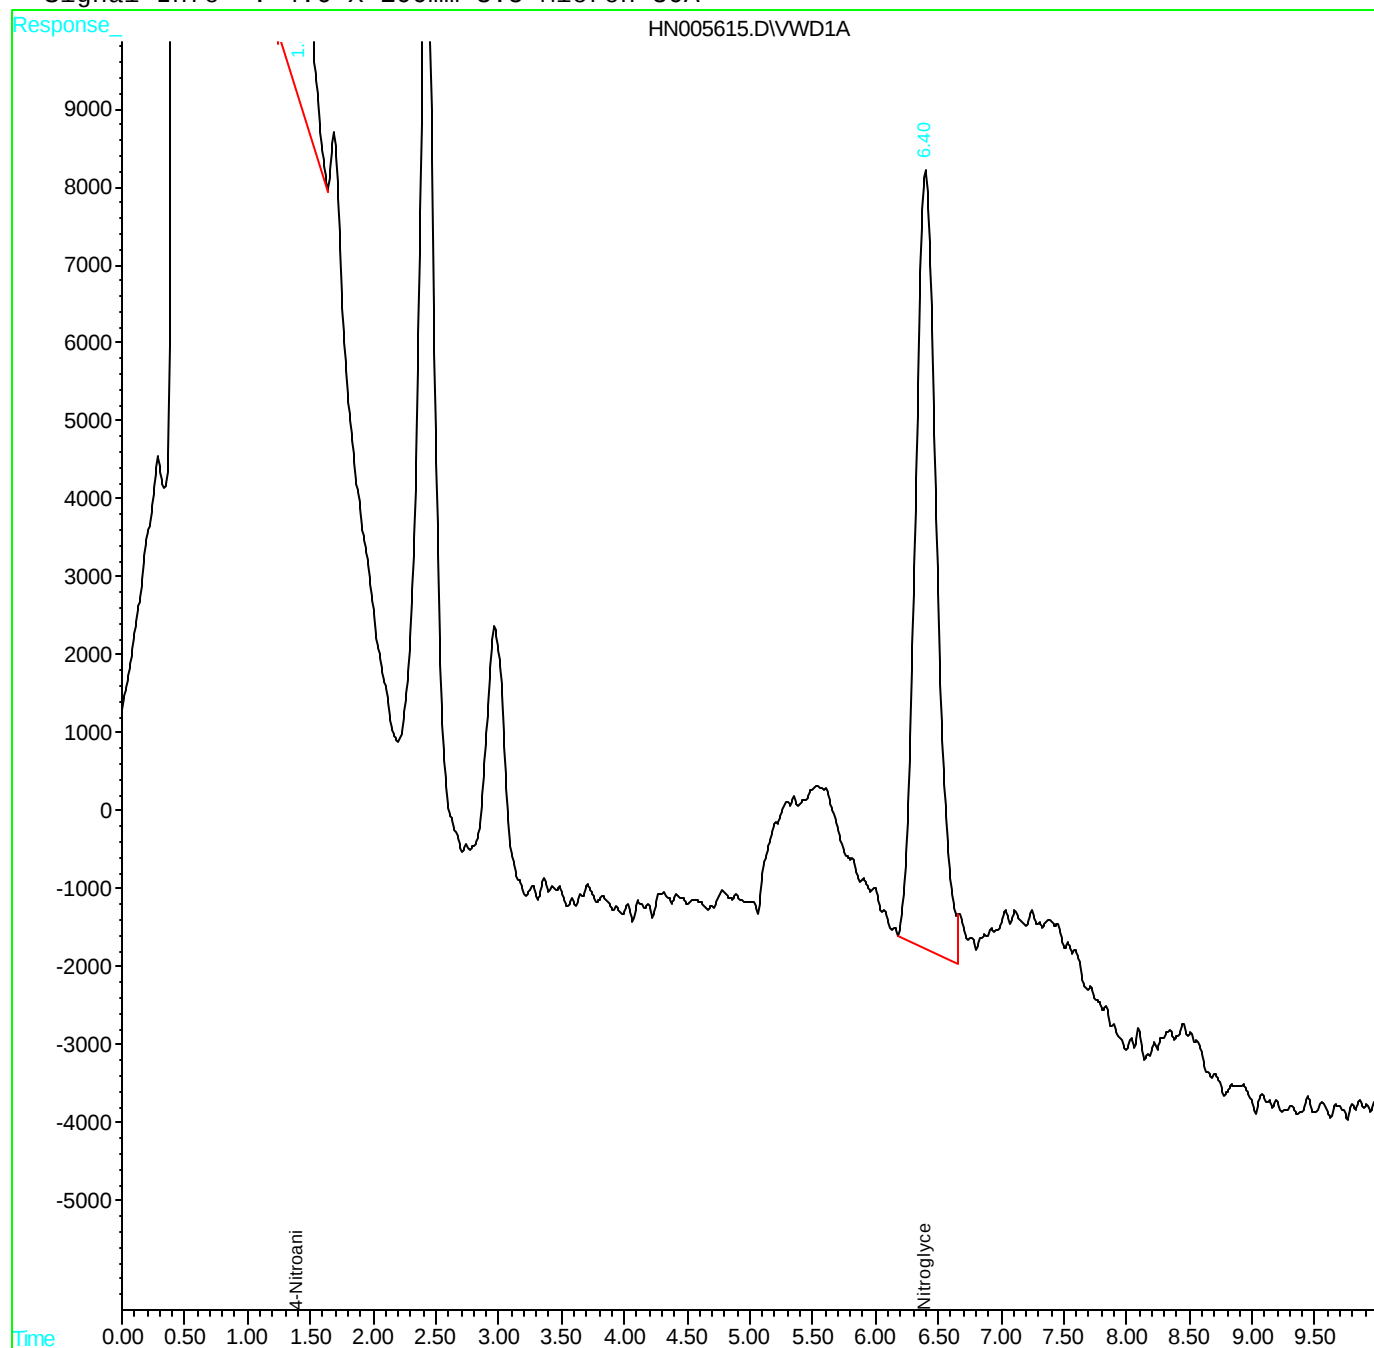


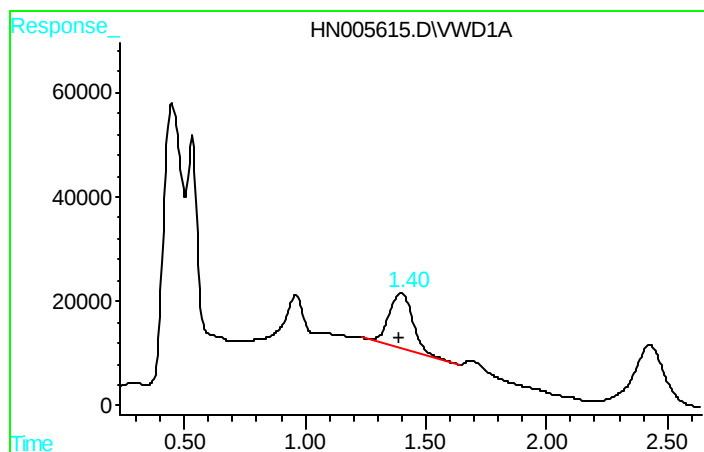

#1 4-Nitroaniline

R.T.: 1.400 min  
 Delta R.T.: 0.010 min  
 Response: 725025  
 Conc: 0.17 ng/ul

Instrument :  
 HPLC\_N  
 ClientSampleId :  
 BG500SS01AMS

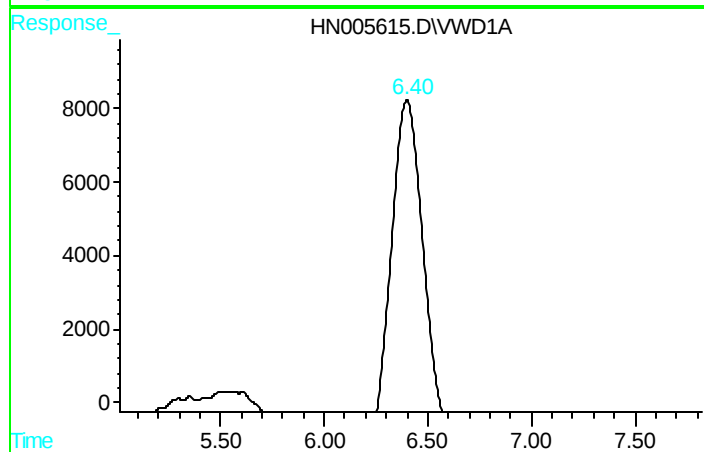

#2 Nitroglycerin

R.T.: 6.401 min  
 Delta R.T.: 0.021 min  
 Response: 1191387  
 Conc: 0.13 ng/ul