

Data File : S:\HPCHEM1\HPLC_N\DATA\HN071113\HN005616.D Vial: 20
Acq On : 11-Jul-2013, 20:55 Operator: QM
Sample : E2837-01MSD Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Jul 12 8:50 2013 Quant Results File: HN071113.RES

Instrument :
HPLC_N
ClientSampleId :
BG500SS01AMSD

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN071113.M
Title :
Last Update : Fri Jul 12 08:34:40 2013
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.35	679484	0.157 ng/ulm

Target Compounds

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005616.D HN071113.M Fri Jul 12 23:44:59 2013 RPT1


Quantitation Report


Data File : S:\HPCHEM1\HPLC_N\DATA\HN071113\HN005616.D Vial: 20
Acq On : 11-Jul-2013, 20:55 Operator: QM
Sample : E2837-01MSD Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Jul 12 8:50 2013 Quant Results File: HN071113.RES

Instrument :
HPLC_N
ClientSampleId :
BG500SS01AMSD

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN071113.M
Title :
Last Update : Fri Jul 12 08:34:40 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

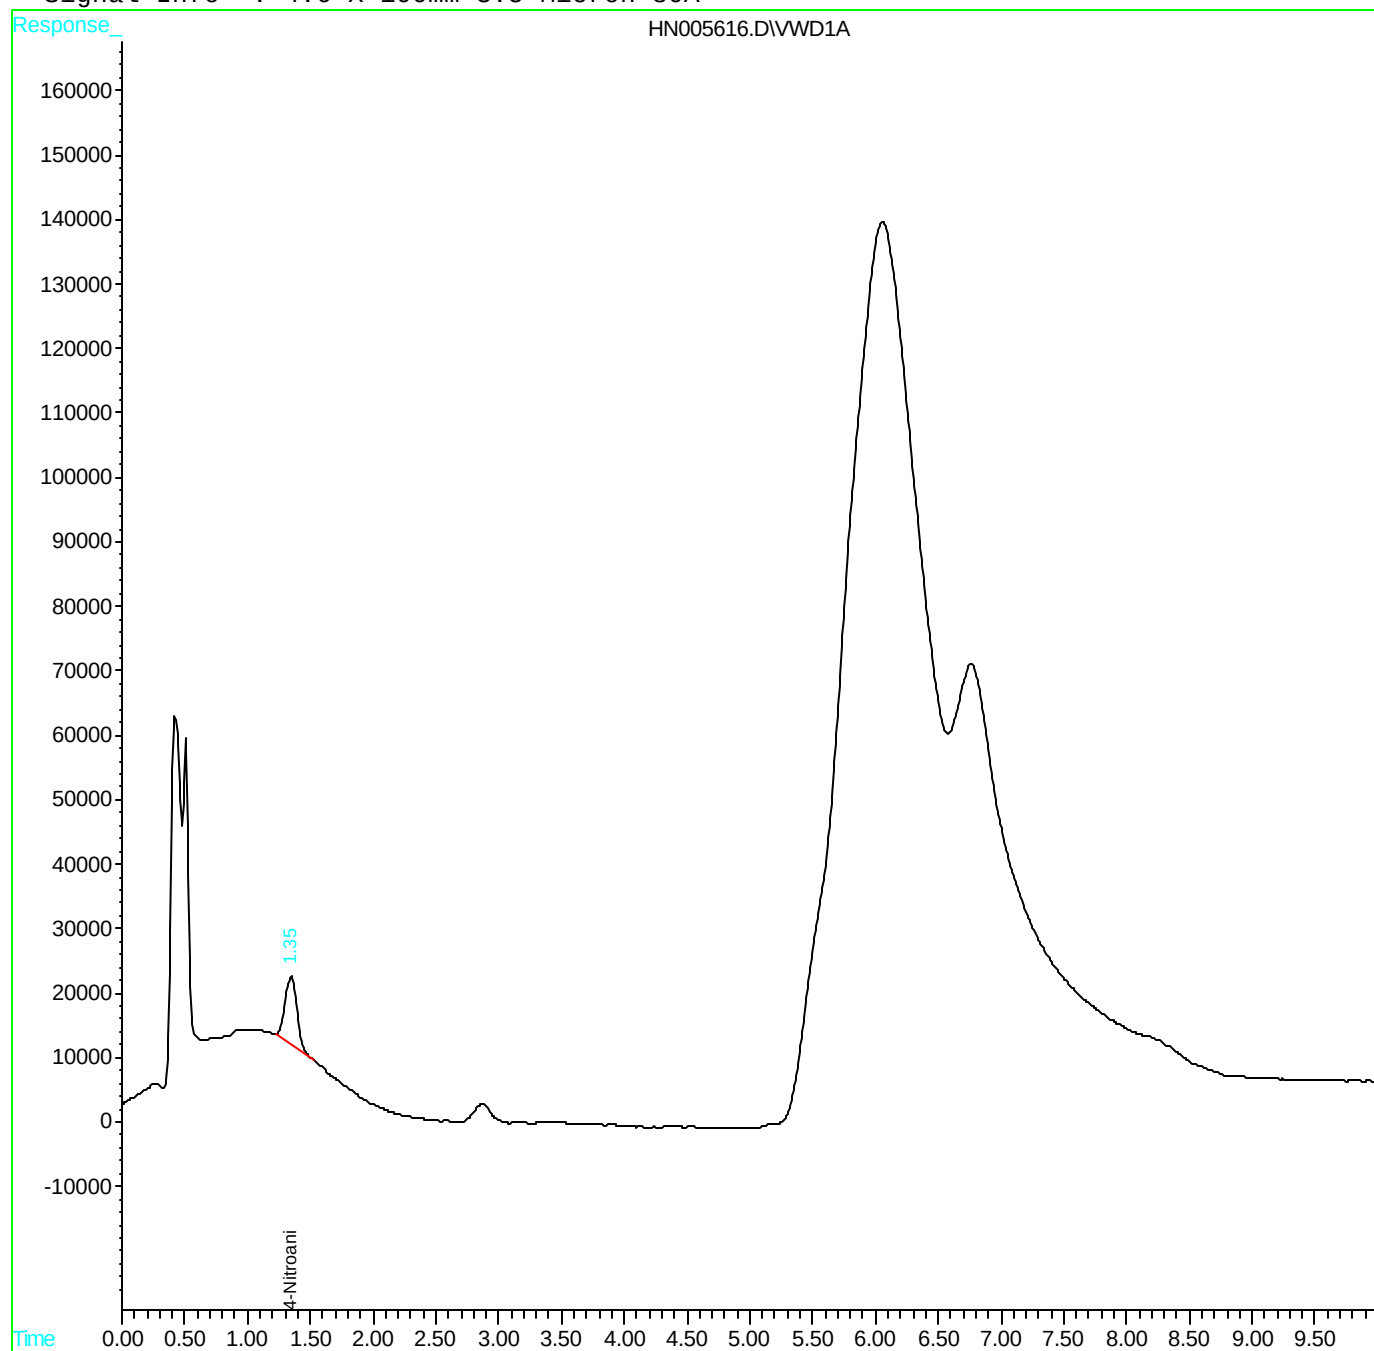

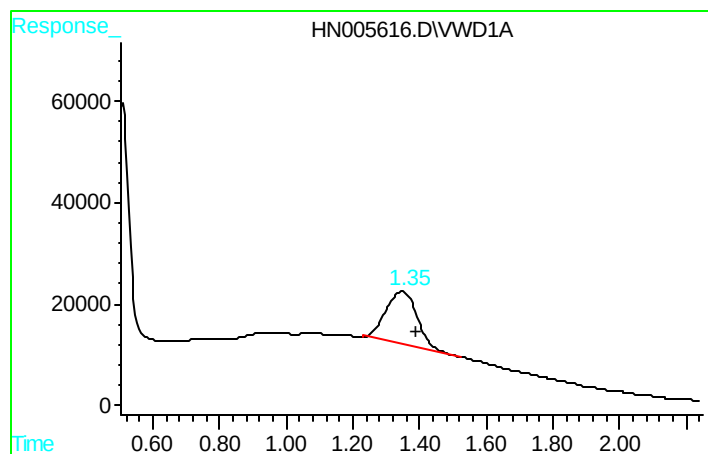

#1 4-Nitroaniline

R.T.: 1.353 min
Delta R.T.: -0.037 min
Response: 679484
Conc: 0.16 ng/ul m

Instrument :
HPLC_N
ClientSampleId :
BG500SS01AMSD