

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN073015\
Data File : HN007445.D
Signal(s) : vwd1A.ch
Acq On : 30-Jul-2015, 17:49
Operator : TP/IZ
Sample : SSTDICC050
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
SSTDICC050

Integration File: AUTOINT1.E
Quant Time: Jul 31 03:31:57 2015
Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN0730NG.M
Quant Title :
QLast Update : Fri Jul 31 03:30:47 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.311	197601134	47.428 ng/ul
Target Compounds			
2) T Nitroglycerin	5.892	403002798	49.345 ng/ul

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN073015\
Data File : HN007445.D
Signal(s) : vwd1A.ch
Acq On : 30-Jul-2015, 17:49
Operator : TP/IZ
Sample : SSTDICC050
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
SSTDICC050

Integration File: AUTOINT1.E
Quant Time: Jul 31 03:31:57 2015
Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN0730NG.M
Quant Title :
QLast Update : Fri Jul 31 03:30:47 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

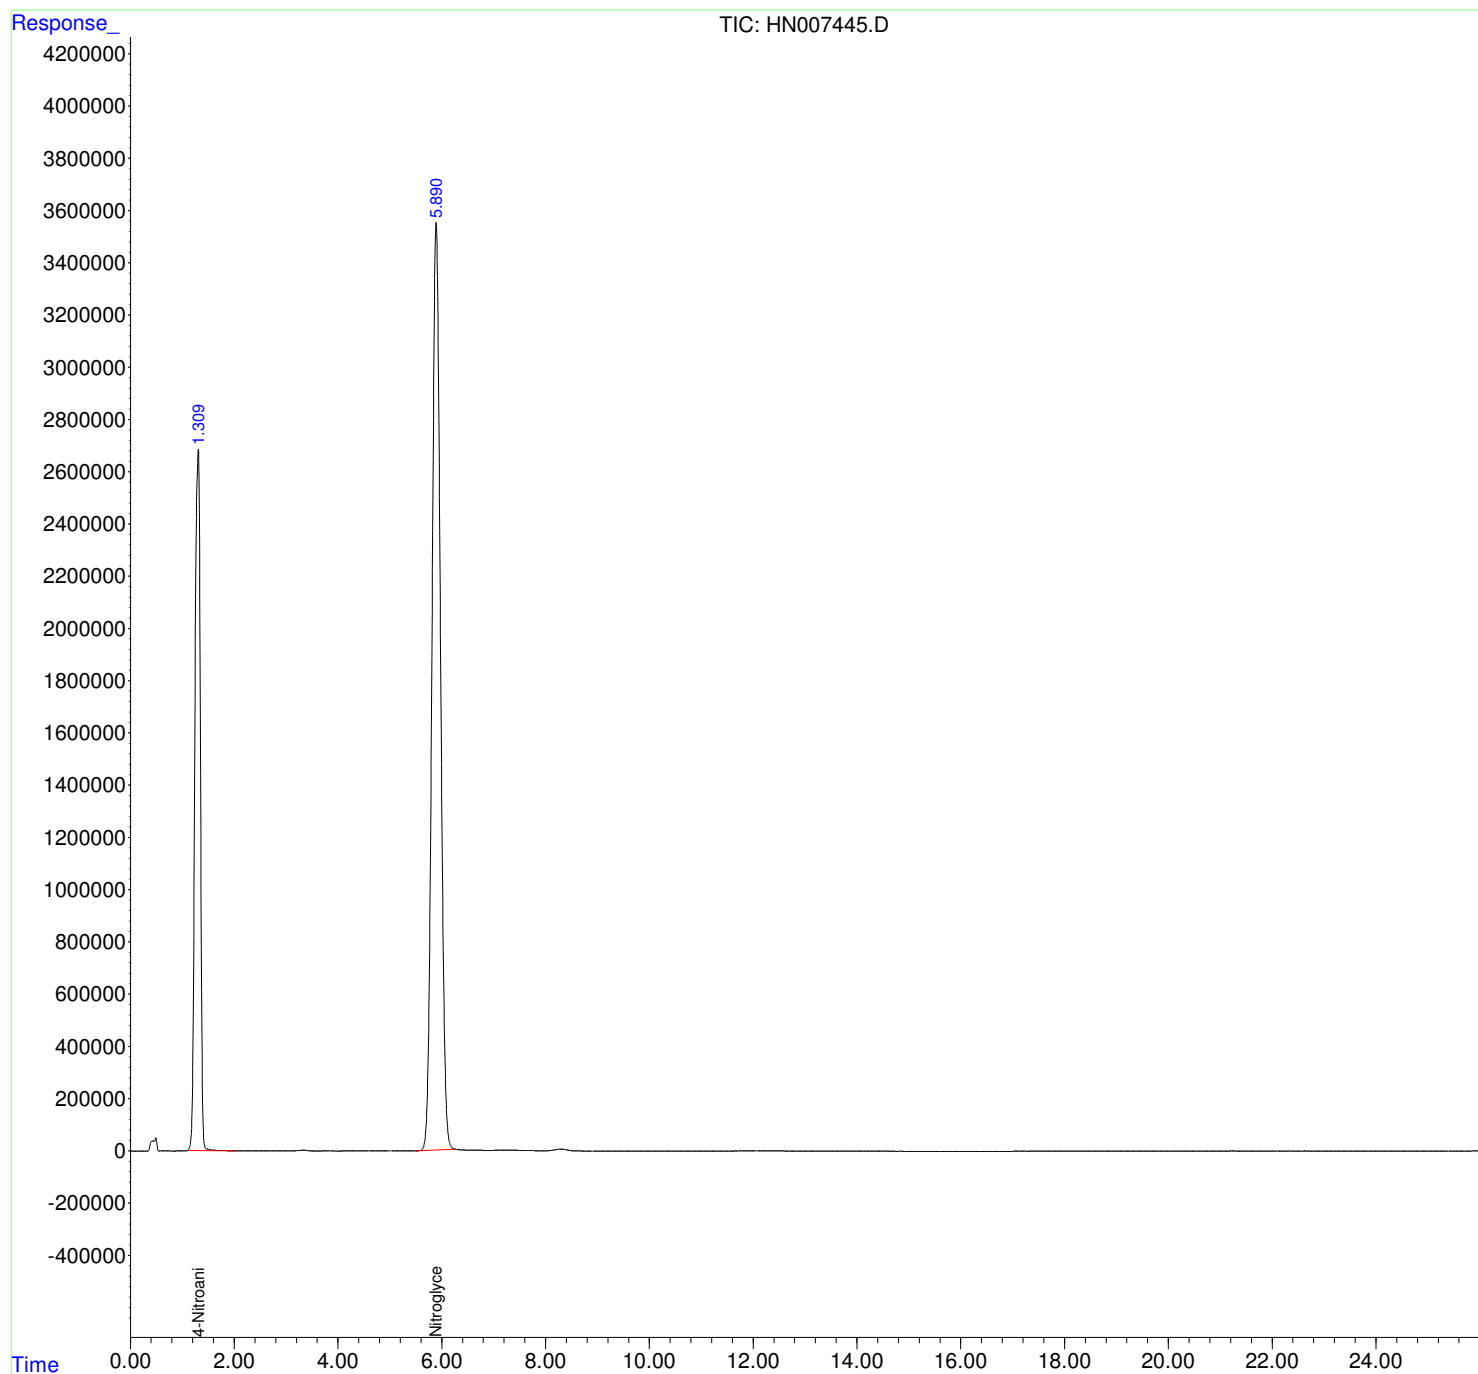


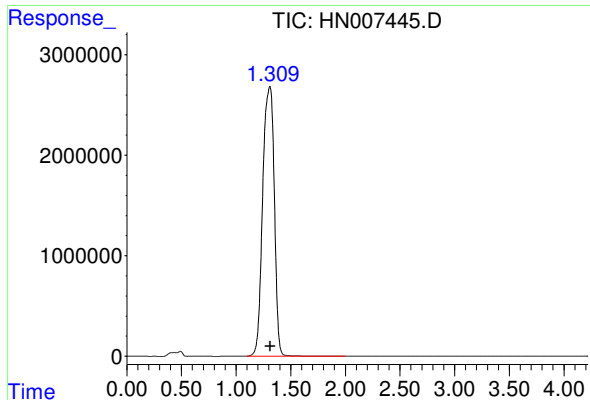

#1 4-Nitroaniline

R.T.: 1.311 min
Delta R.T.: -0.001 min
Response: 197601134
Conc: 47.43 ng/u1

Instrument :
HPLC_N
ClientSampleId :
SSTDIC050

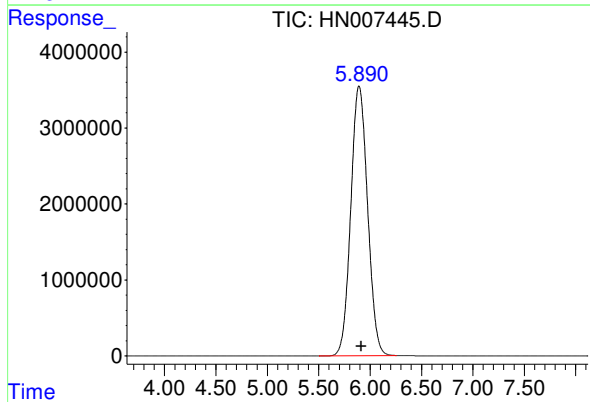

#2 Nitroglycerin

R.T.: 5.892 min
Delta R.T.: -0.021 min
Response: 403002798
Conc: 49.34 ng/u1