

Signal #1 : S:\HPCHEM1\HPLC_N\DATA\HN081314\HN006232.D\VWD1A.CH Vial:
 Signal #2 : S:\HPCHEM1\HPLC_N\DATA\HN081314\HN006232.D\VWD1A.CH
 Acq On : 13-Aug-2014, 12:26 Operator: HNP
 Sample : F3388-01 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e
 Quant Time: Aug 13 15:29 2014 Quant Results File: HN071714.RES

Instrument :
 HPLC_N
 ClientSampleId :
 HF-OAT-S-01

Manual Integrations
 APPROVED

TEJASKUMAR
 8/14/2014 6:05:46 PM

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN071714.M
 Title :
 Last Update : Fri Aug 08 10:46:30 2014
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.44	623273	141.515 ug/L m

Target Compounds

 Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN006232.D HN071714.M

Fri Aug 15 18:11:09 2014

RPT1

Quantitation Report

Signal #1 : S:\HPCHEM1\HPLC_N\DATA\HN081314\HN006232.D\VWD1A.CH Vial:
Signal #2 : S:\HPCHEM1\HPLC_N\DATA\HN081314\HN006232.D\VWD1A.CH
Acq On : 13-Aug-2014, 12:26 Operator: HNP
Sample : F3388-01 Inst : G1314A
Misc : Multiplr: 1.00
IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e
Quant Time: Aug 13 15:29 2014 Quant Results File: HN071714.RES



Instrument :
HPLC_N
ClientSampleId :
HF-OAT-S-01


Manual Integrations
APPROVED

TEJASKUMAR
8/14/2014 6:05:46 PM

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN071714.M
Title :
Last Update : Fri Aug 08 10:46:30 2014
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

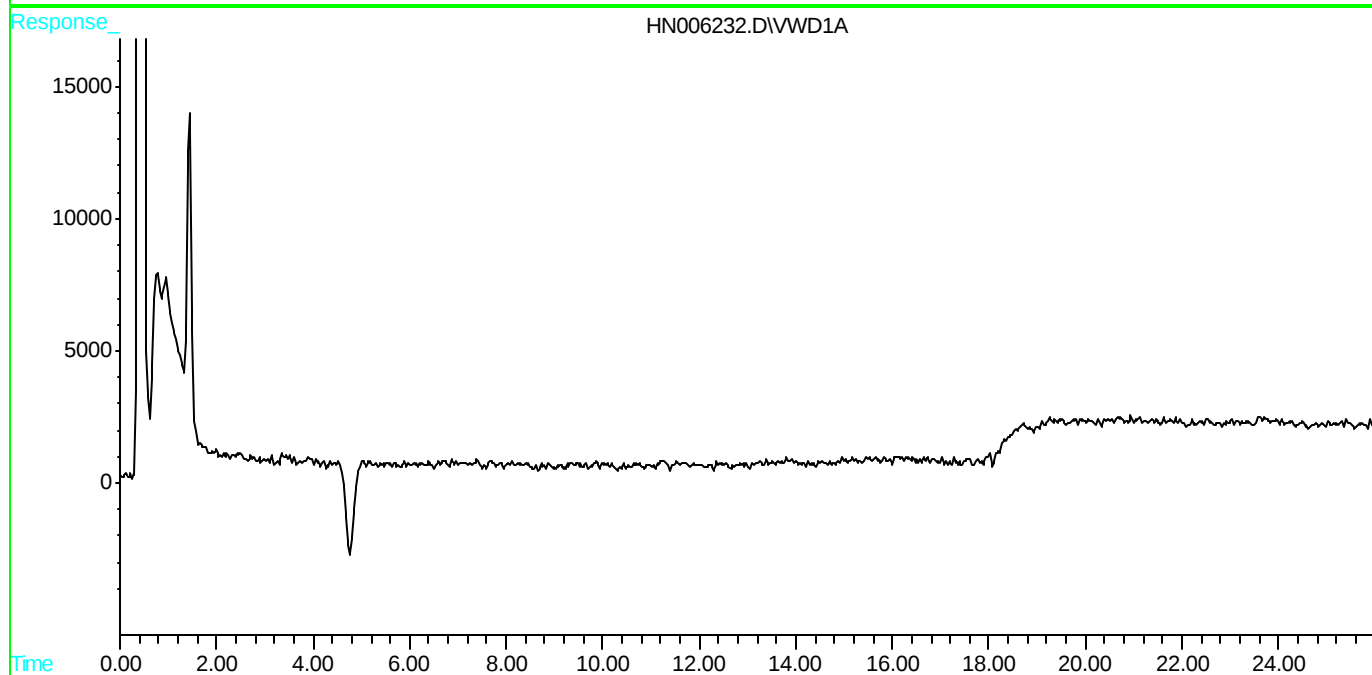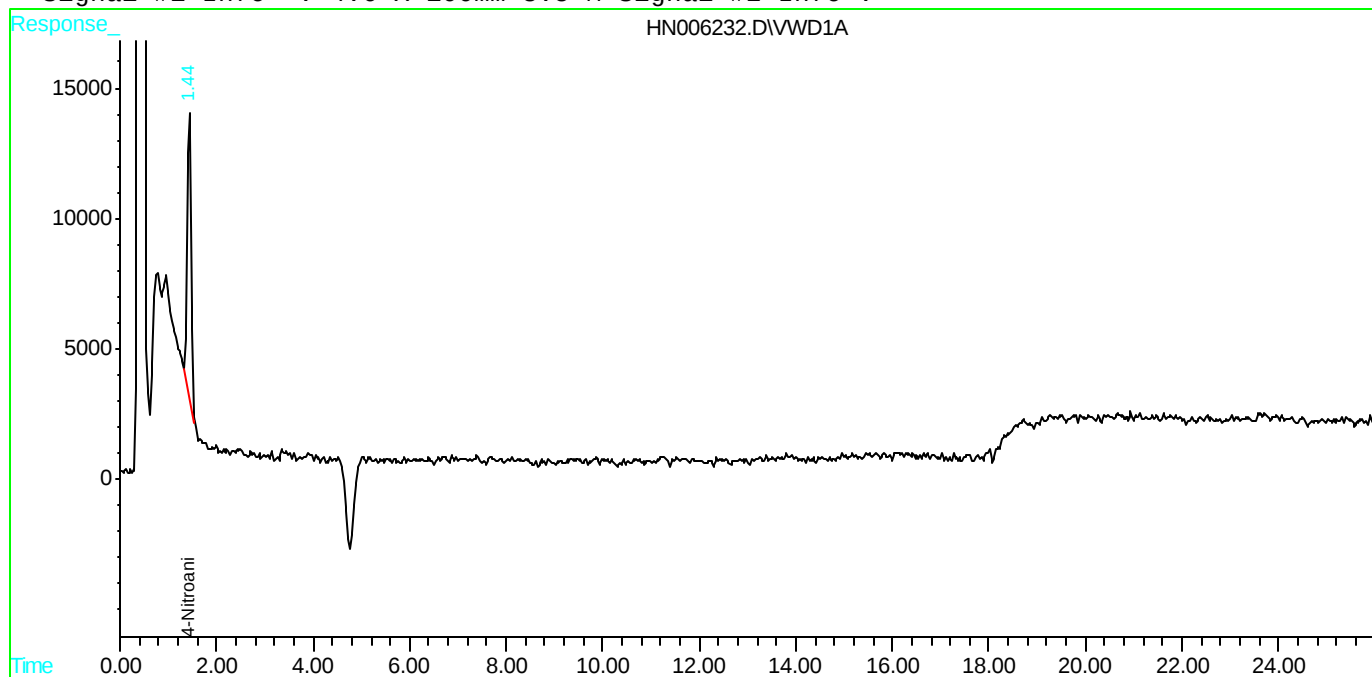

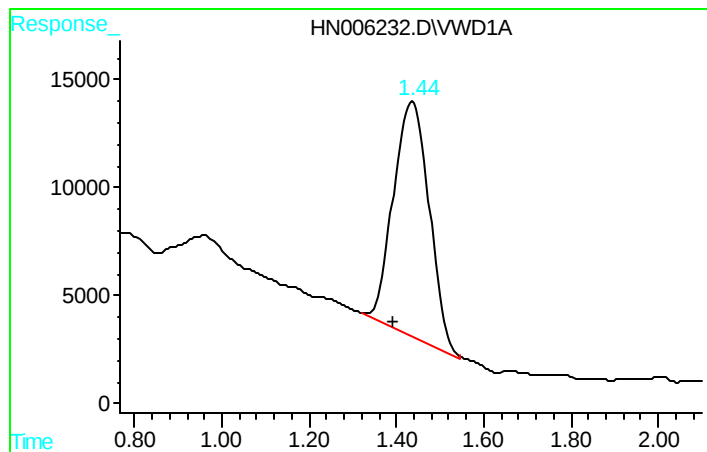

#1 4-Nitroaniline

R.T.: 1.436 min
Delta R.T.: 0.046 min
Response: 623273
Conc: 141.51 ug/L m

Instrument :
HPLC_N
ClientSampleId :
HF-OAT-S-01

Manual Integrations
APPROVED

TEJASKUMAR
8/14/2014 6:05:46 PM