

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN081315\
 Data File : HN007505.D
 Signal(s) : vwd1A.ch
 Acq On : 13-Aug-2015, 12:37
 Operator : TP/IZ
 Sample : SSTDICC2000
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 14 11:41:21 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN081315.M
 Quant Title :
 QLast Update : Fri Aug 14 11:37:02 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.356	3780938	879.214 ug/L
Target Compounds			
2) T HMX	0.908	4837531	958.733 ug/L
3) T RDX	1.749	5397532	865.263 ug/L
4) T 1,3,5-Trinitrobenzene	2.714	11343157	872.276 ug/L
5) T 1,3-Dinitrobenzene	3.611	17304983	891.552 ng/ml
6) T 3,5-Dinitroaniline	4.020	13427982	929.730 ug/L
7) T Nitrobenzene	4.846f	9729199	837.610 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN081315\
Data File : HN007505.D
Signal(s) : vwd1A.ch
Acq On : 13-Aug-2015, 12:37
Operator : TP/IZ
Sample : SSTDICC2000
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 14 11:41:21 2015
Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN081315.M
Quant Title :
QLast Update : Fri Aug 14 11:37:02 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

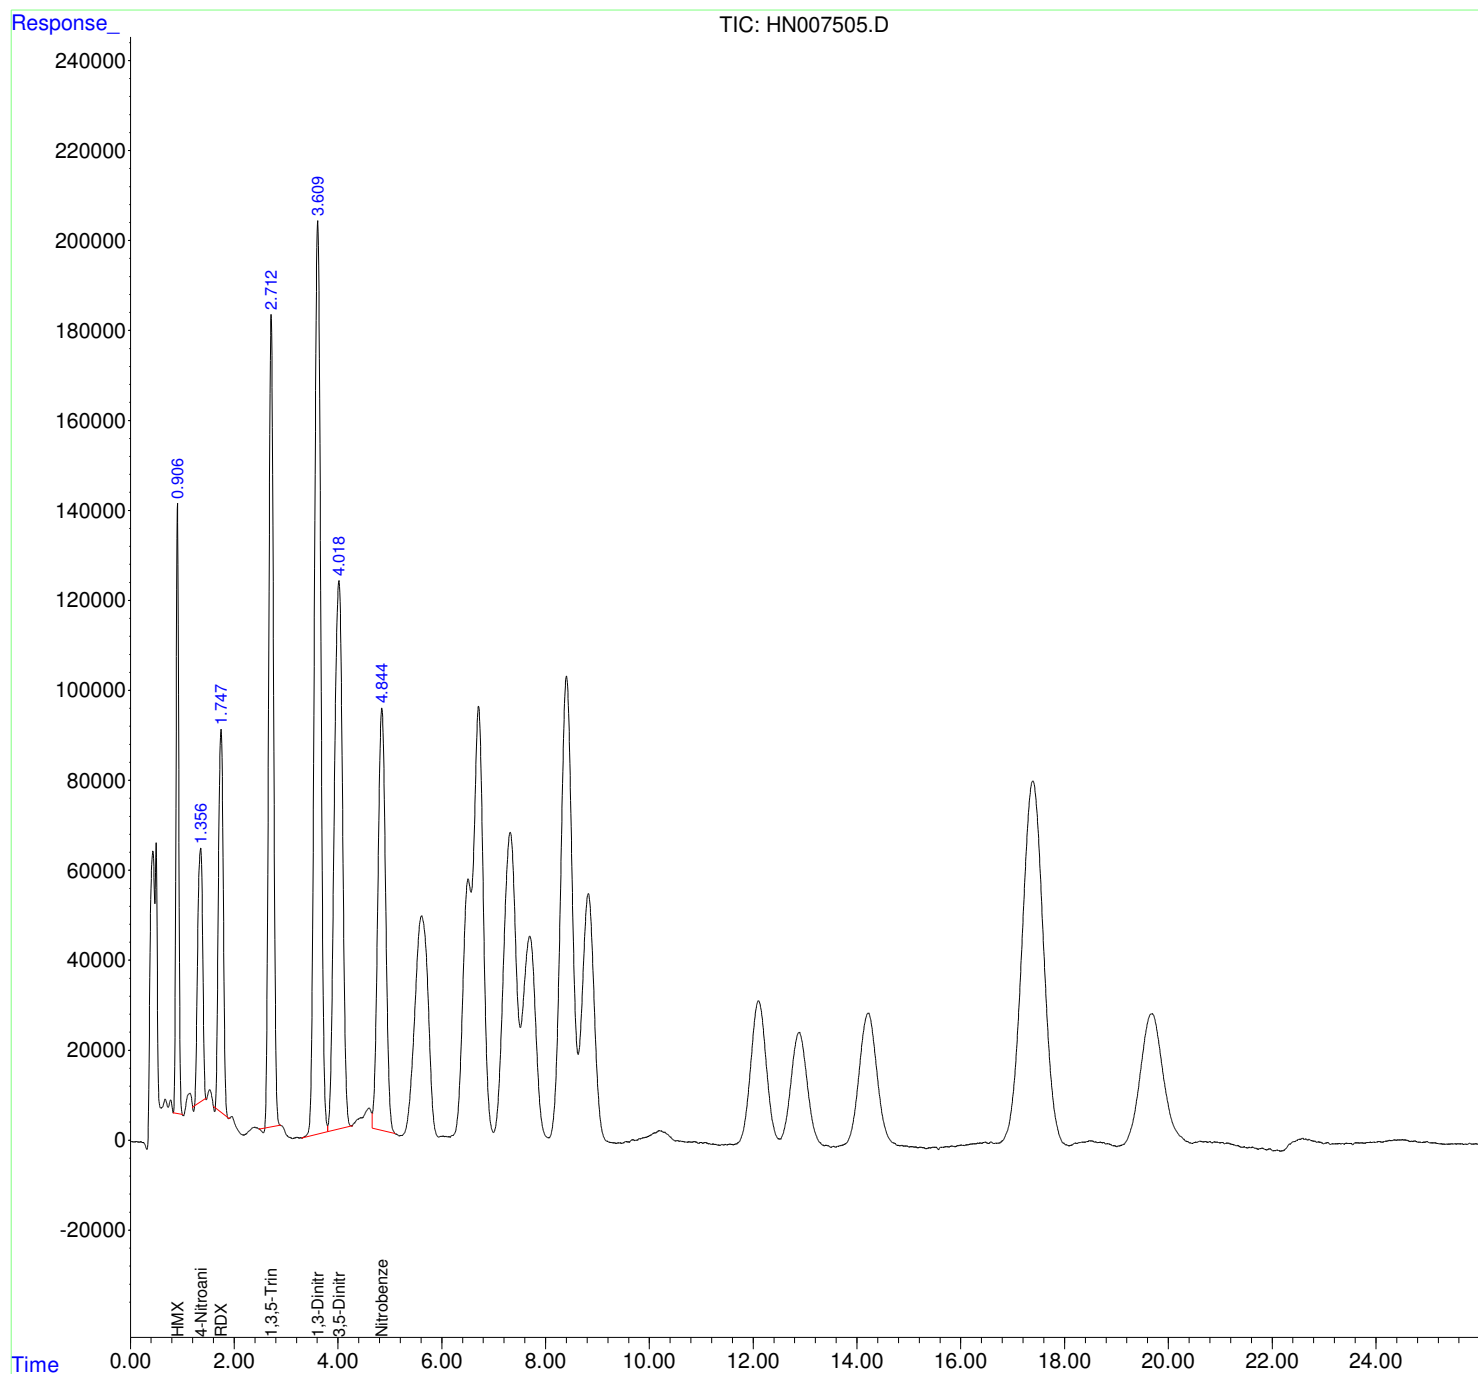


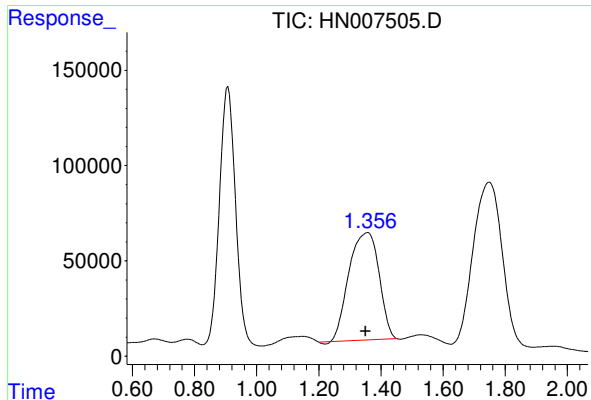

#1 4-Nitroaniline


R.T.: 1.356 min
Delta R.T.: 0.005 min
Response: 3780938
Conc: 879.21 ug/L

Instrument :
HPLC_N
ClientSampleId :

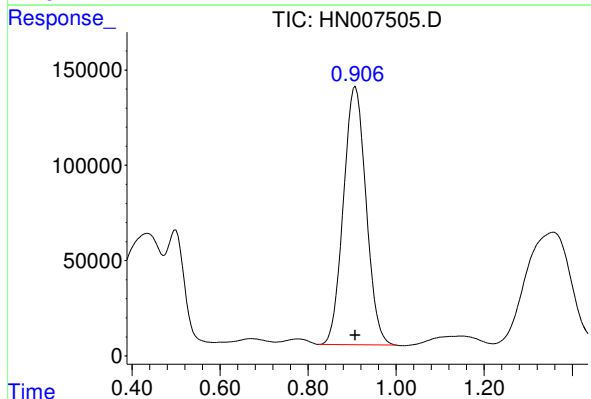


#2 HMX

R.T.: 0.908 min
Delta R.T.: 0.001 min
Response: 4837531
Conc: 958.73 ug/L

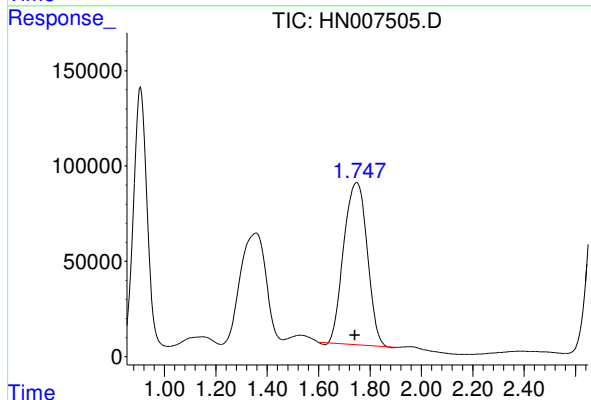


#3 RDX

R.T.: 1.749 min
Delta R.T.: 0.008 min
Response: 5397532
Conc: 865.26 ug/L

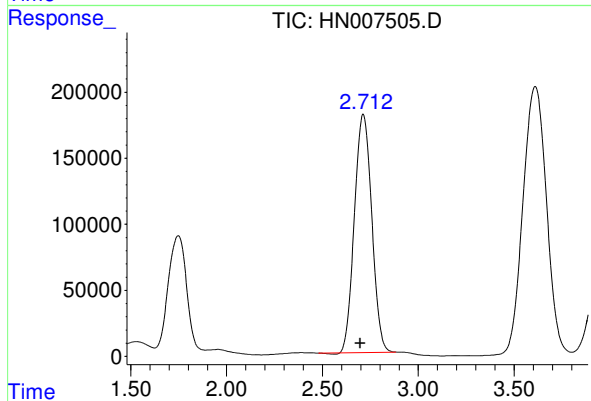

#4 1,3,5-Trinitrobenzene


R.T.: 2.714 min
Delta R.T.: 0.017 min
Response: 11343157
Conc: 872.28 ug/L

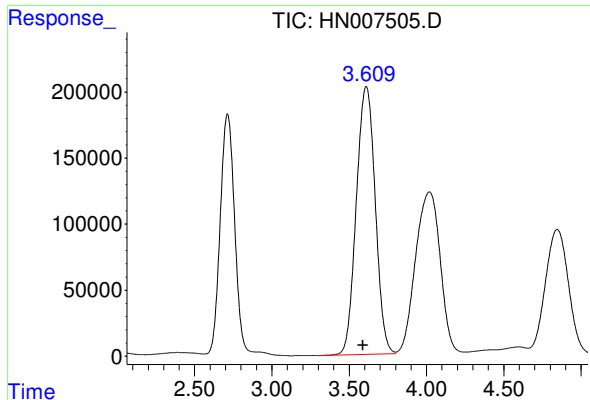

#5 1,3-Dinitrobenzene


R.T.: 3.611 min
Delta R.T.: 0.023 min
Response: 17304983
Conc: 891.55 ng/ml

Instrument :
HPLC_N
ClientSampleId :

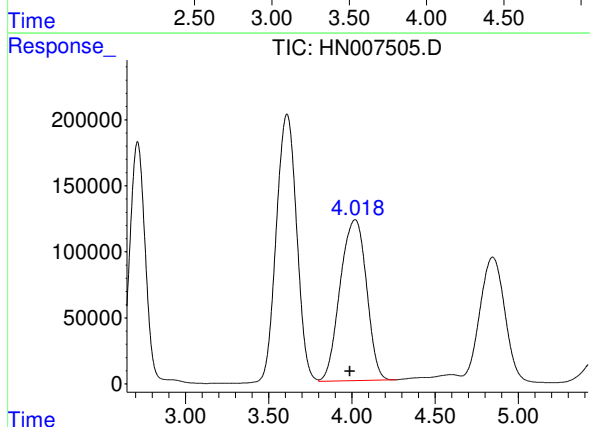

#6 3,5-Dinitroaniline

R.T.: 4.020 min
Delta R.T.: 0.031 min
Response: 13427982
Conc: 929.73 ug/L

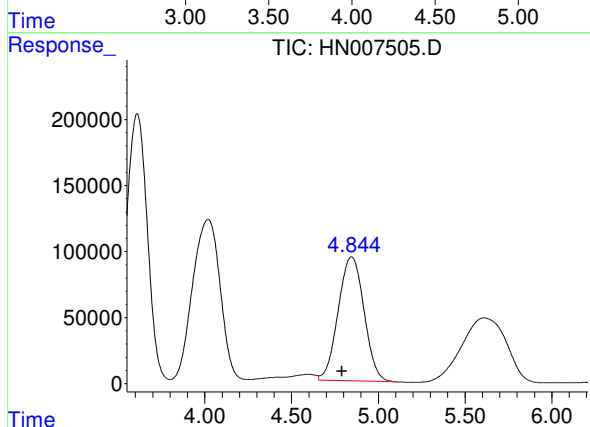

#7 Nitrobenzene

R.T.: 4.846 min
Delta R.T.: 0.055 min
Response: 9729199
Conc: 837.61 ug/L