

Data File : H:\VOL1\HPLC\HPLC N\120815\HN000454.D Vial: 7
Acq On : 15-Aug-2012, 19:34 Operator: HLM
Sample : 8330-MRL Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Aug 16 10:31 2012 Quant Results File: HN081512.RES

Quant Method : H:\VOL1\HPLC\HPLC N\METHODS\HN081512.M (Chemstation Integrator)
Title : SW8330 / 8330A confirmation
Last Update : Thu Aug 16 10:32:50 2012
Response via : Initial Calibration
DataAcq Meth : 8330VWDC.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds


3) T	RDX	10.44f	243598	18.092 ug/L
7) T	2-Amino-4,6-dinitrotoluene	15.66	431128	9.066 ug/L
8) T	4-Amino-2,6-dinitrotoluene	15.66	431128	9.066 ug/L
9) T	2,4-Dinitrotoluene	21.01f	338016	8.966 ug/L
11) T	1,3-Dinitrobenzene	15.30f	357328	9.354 ug/L
12) T	Nitrobenzene	11.93f	268486	10.265 ug/L
16) T	3,5-Dinitroaniline	13.24f	665676	19.860 ug/L


Quantitation Report

Data File : H:\VOL1\HPLC\HPLC N\120815\HN000454.D Vial: 7
 Acq On : 15-Aug-2012, 19:34 Operator: HLM
 Sample : 8330-MRL Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Aug 16 10:31 2012 Quant Results File: HN081512.RES

Quant Method : H:\VOL1\HPLC\HPLC N\METHODS\HN081512.M (Chemstation Integrator)
 Title : SW8330 / 8330A confirmation
 Last Update : Thu Aug 16 10:32:50 2012
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330VWDC.M


Volume Inj. :
 Signal Phase :
 Signal Info :

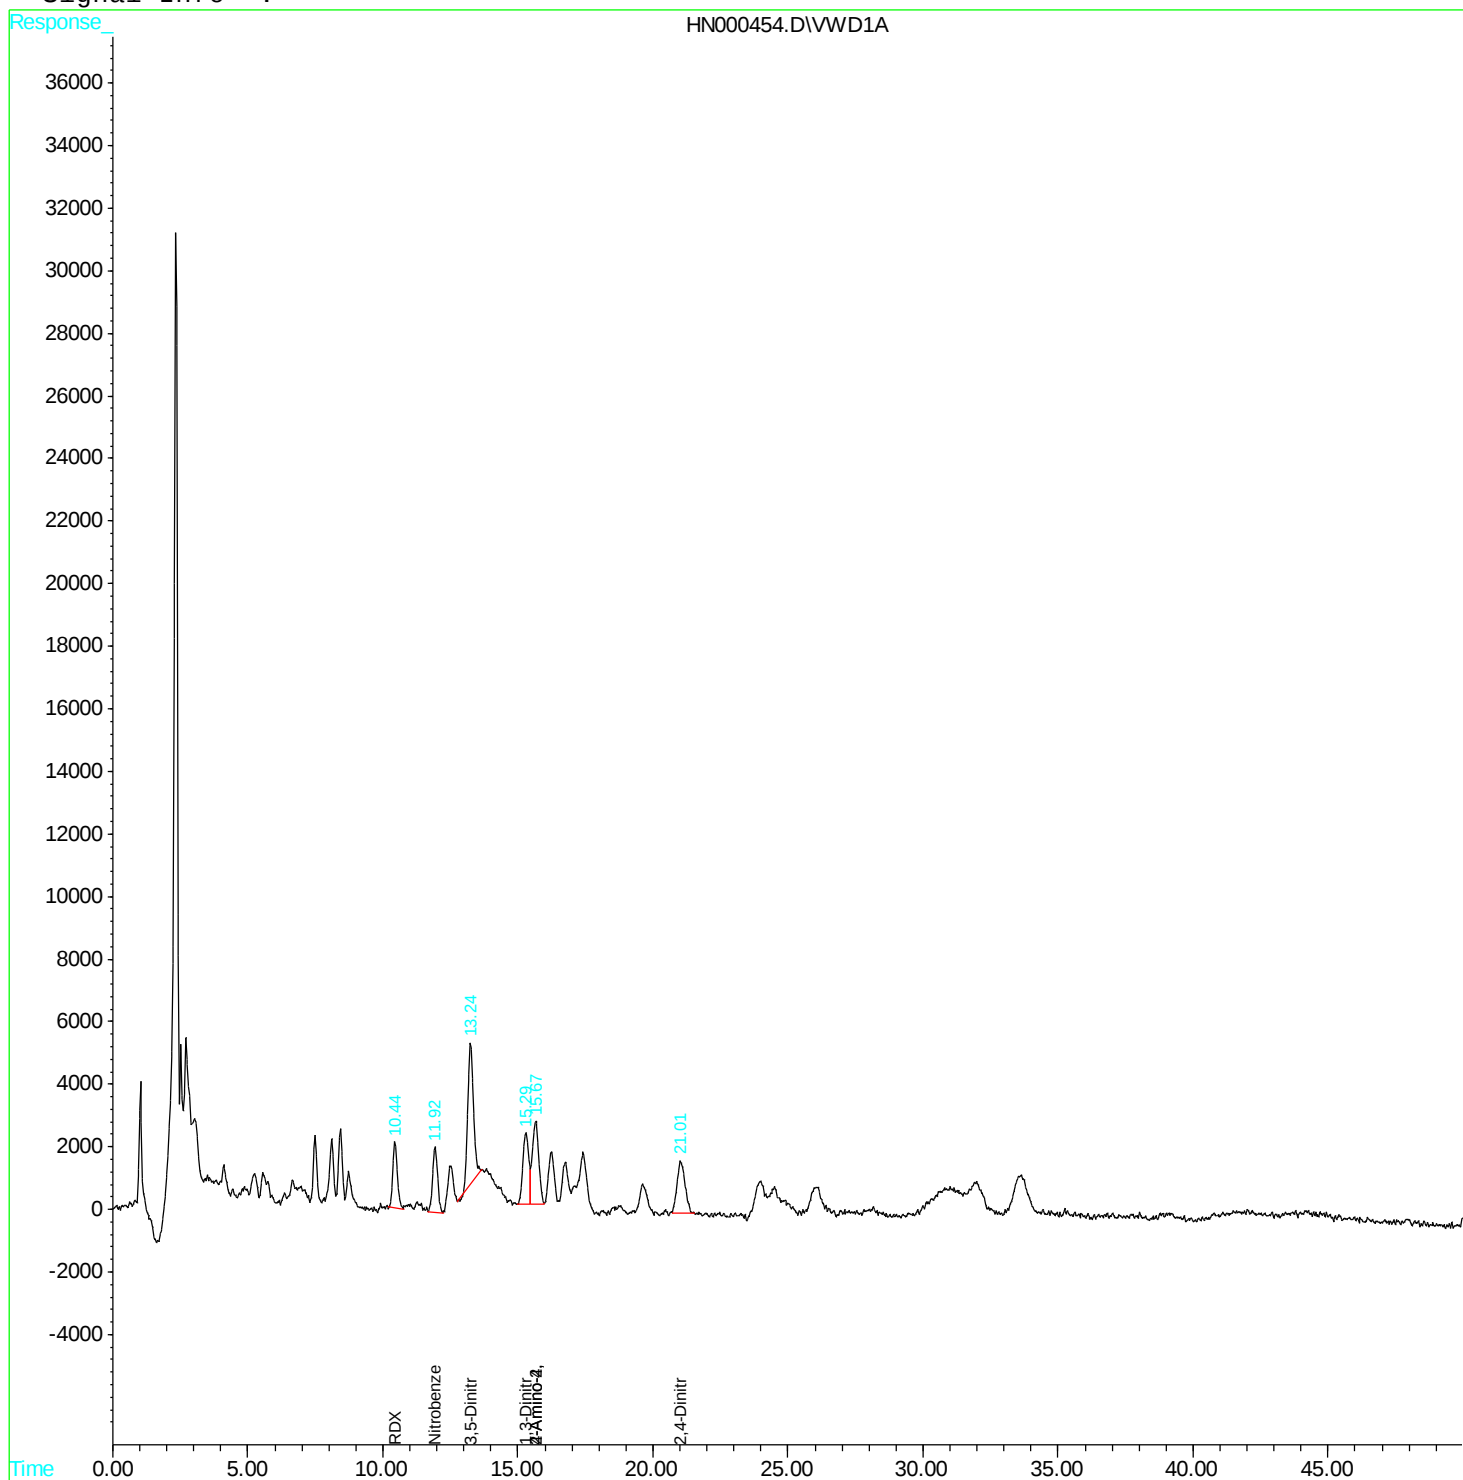

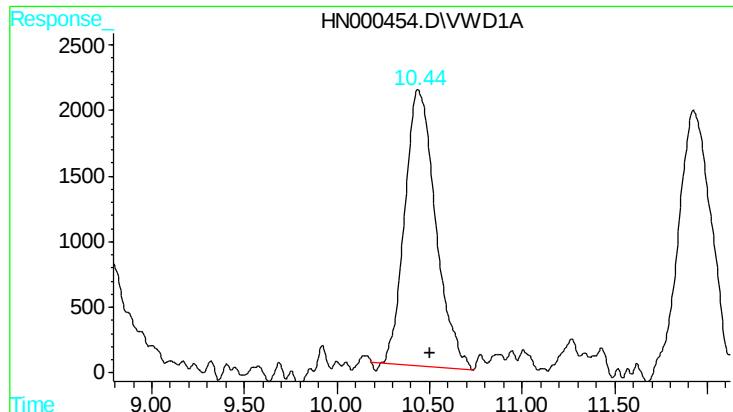


#3 RDX

R.T.: 10.438 min
Delta R.T.: -0.065 min
Response: 243598
Conc: 18.09 ug/L

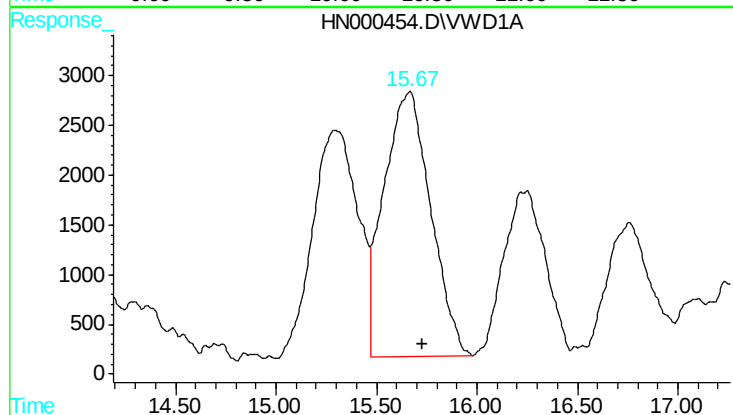


#7 2-Amino-4,6-dinitrotoluene

R.T.: 15.662 min
Delta R.T.: -0.070 min
Response: 431128
Conc: 9.07 ug/L

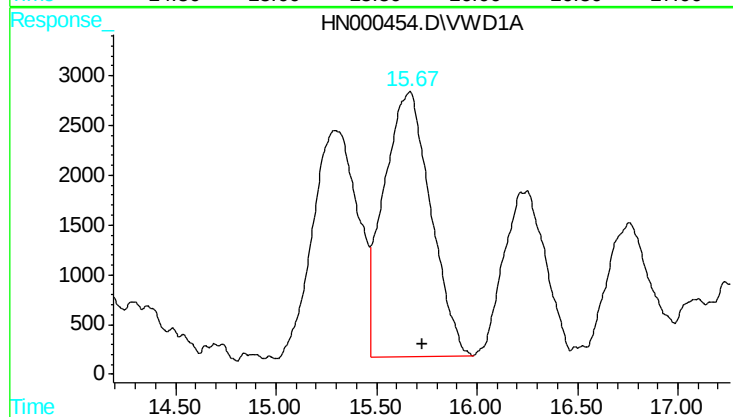


#8 4-Amino-2,6-dinitrotoluene

R.T.: 15.662 min
Delta R.T.: -0.070 min
Response: 431128
Conc: 9.07 ug/L

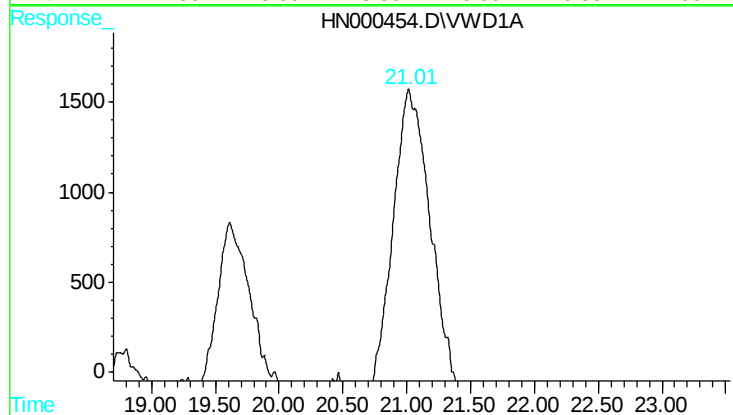


#9 2,4-Dinitrotoluene

R.T.: 21.014 min
Delta R.T.: -0.125 min
Response: 338016
Conc: 8.97 ug/L

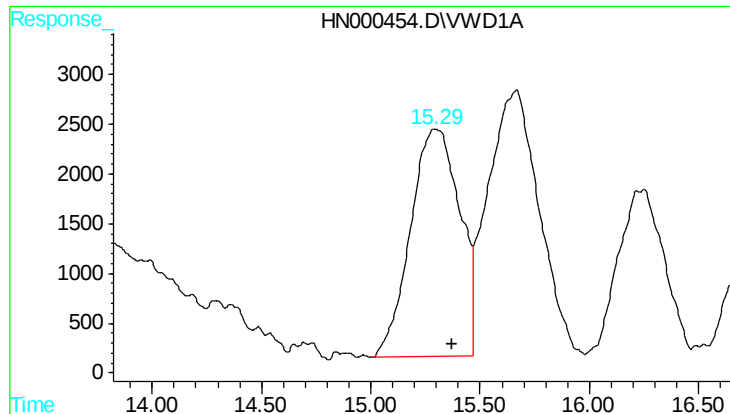


#11 1,3-Dinitrobenzene

R.T.: 15.299 min
Delta R.T.: -0.074 min
Response: 357328
Conc: 9.35 ug/L

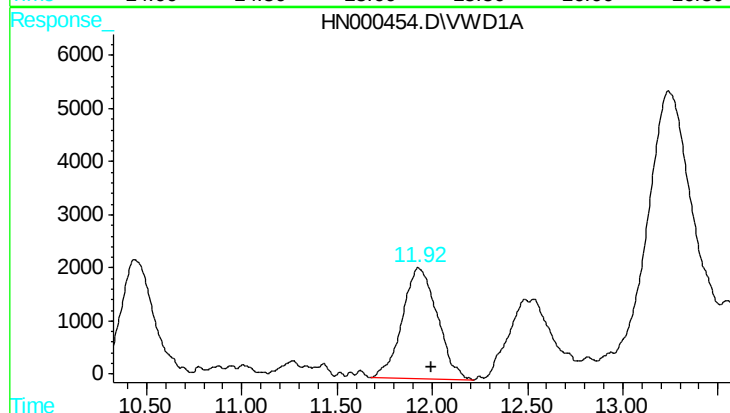

#12 Nitrobenzene

R.T.: 11.927 min
Delta R.T.: -0.070 min
Response: 268486
Conc: 10.26 ug/L

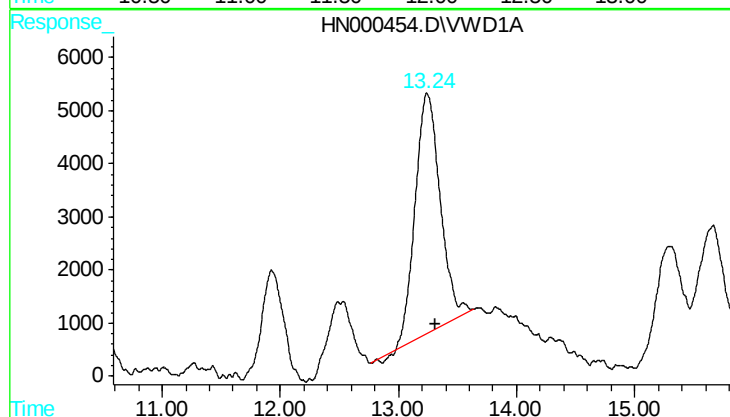

#16 3,5-Dinitroaniline

R.T.: 13.241 min
Delta R.T.: -0.068 min
Response: 665676
Conc: 19.86 ug/L