

Data Path : S:\HPCHEM1\HPLC_N\Data\HN090512\
Data File : HN000465.D
Signal(s) : VWD1A.CH
Acq On : 05-Sep-2012, 20:19
Operator : HLM
Sample : 8330S-LOD1
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
HPLC_N
ClientSampleId :
8330S-LOD1


Manual Integrations
APPROVED

AHPatel
9/11/2012 5:08:04 AM

Integration File: events.e
Quant Time: Sep 07 02:28:59 2012
Quant Method : S:\HPCHEM1\HPLC_N\Method\HN081512.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Thu Aug 16 10:32:31 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

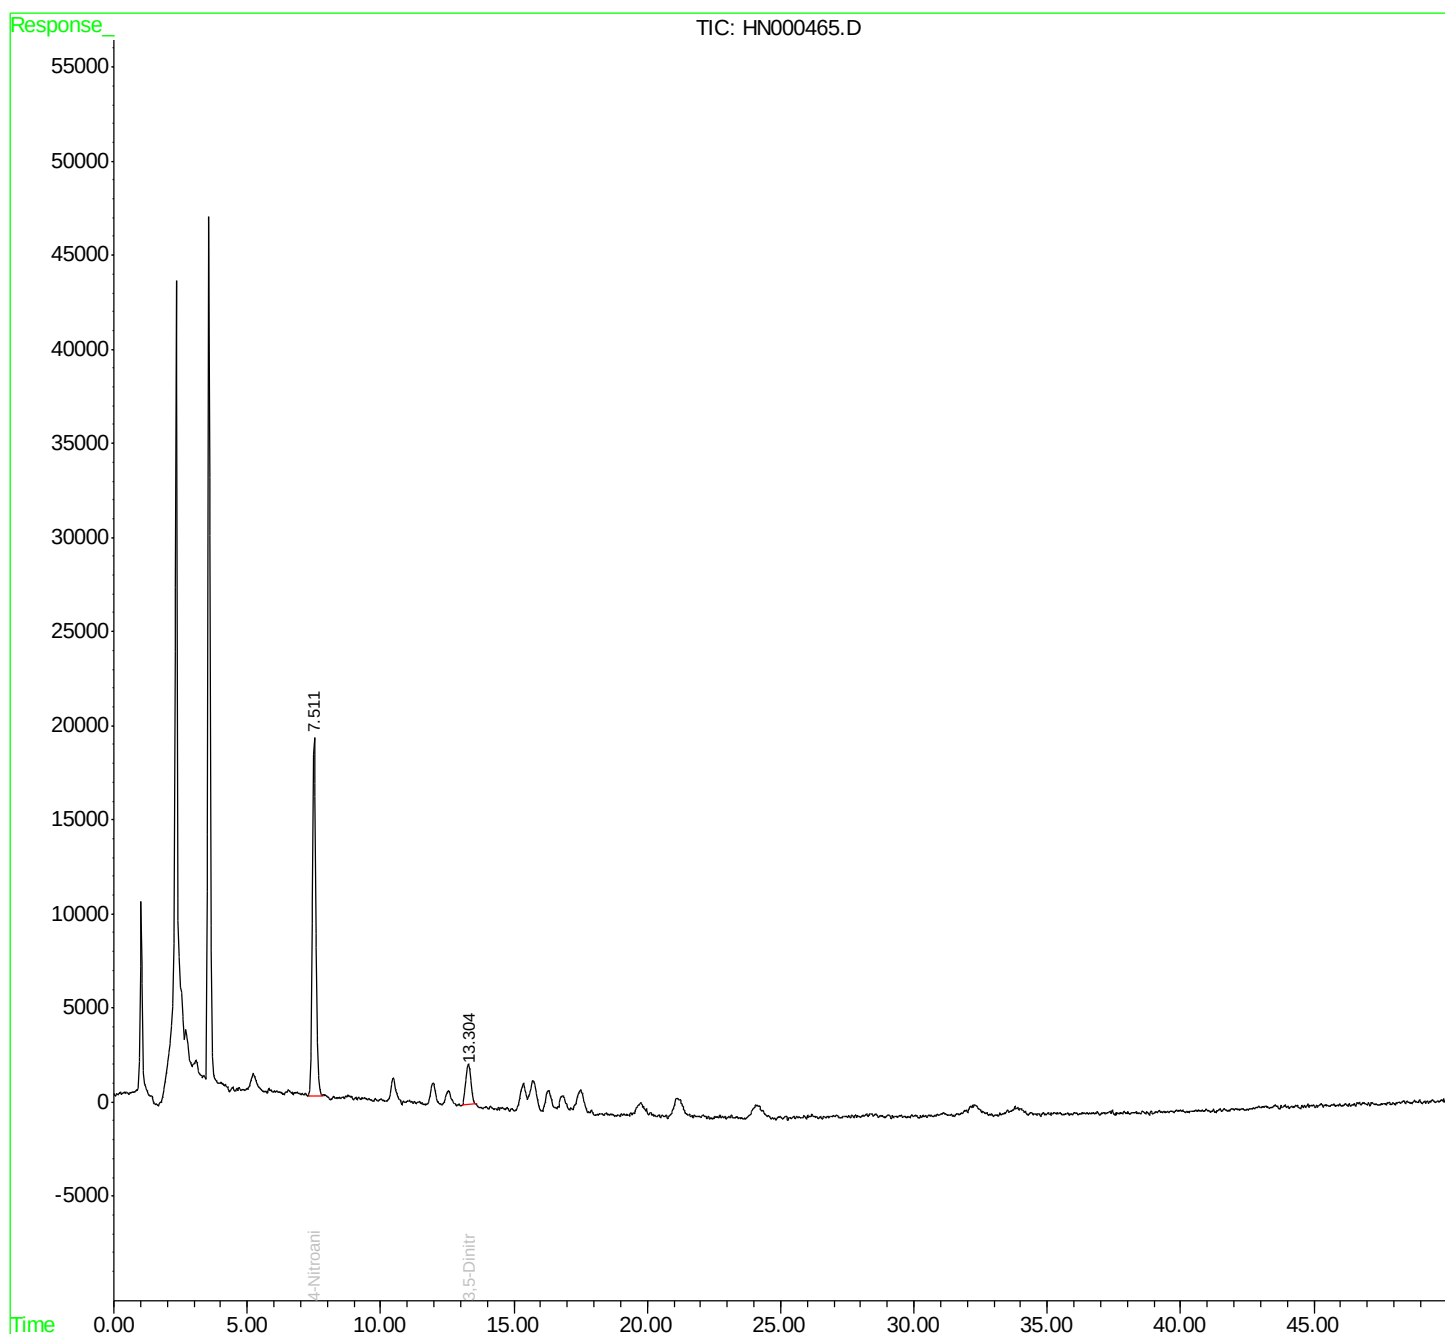

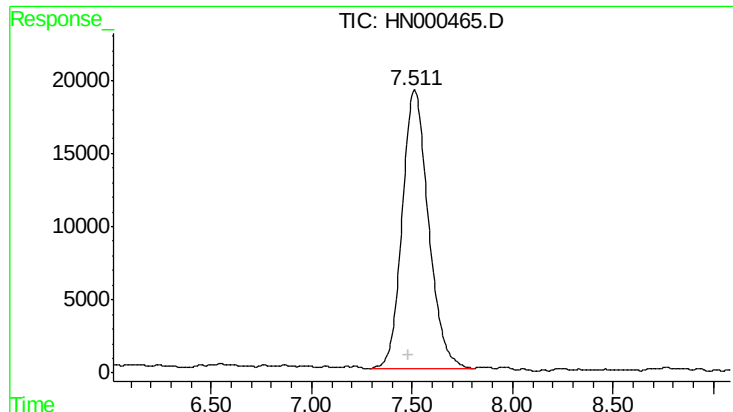


#1 4-Nitroaniline

R.T.: 7.513 min
Delta R.T.: 0.030 min
Response: 1723854
Conc: 175.12 ug/L

Instrument :
HPLC_N
ClientSampleId :
8330S-LOD1

Manual Integrations
APPROVED

AHPatel
9/11/2012 5:08:04 AM

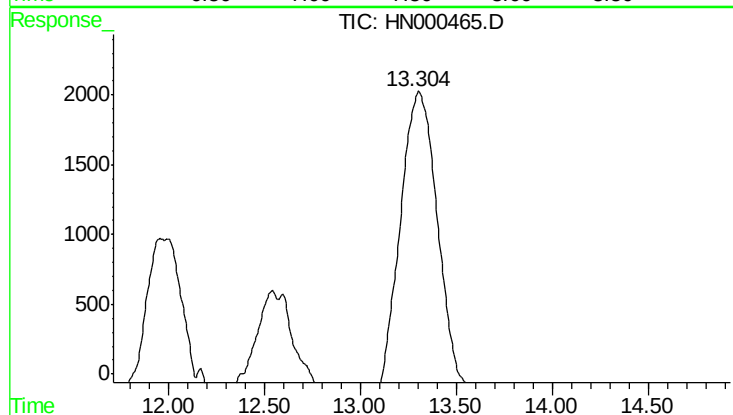

#16 3,5-Dinitroaniline

R.T.: 13.306 min
Delta R.T.: 0.079 min
Response: 286033
Conc: 8.53 ug/L

Data Path : S:\HPCHEM1\HPLC_N\Data\HN090512\
Data File : HN000465.D
Signal(s) : VWD1A.CH
Acq On : 05-Sep-2012, 20:19
Operator : HLM
Sample : 8330S-LOD1
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
8330S-LOD1

Manual Integrations
APPROVED

AHPatel
9/11/2012 5:08:04 AM

Integration File: events.e
Quant Time: Sep 07 02:28:59 2012
Quant Method : S:\HPCHEM1\HPLC_N\Method\HN081512.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Thu Aug 16 10:32:31 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
1) S	4-Nitroaniline	7.513f	1723854	175.123 ug/L
Target Compounds				
16) T	3,5-Dinitroaniline	13.306f	286033	8.533 ug/L

(f)=RT Delta > 1/2 Window

(m)=manual int.