

Data Path : S:\HPCHEM1\HPLC_N\Data\HN090512\
Data File : HN000467.D
Signal(s) : VWD1A.CH
Acq On : 05-Sep-2012, 22:04
Operator : HLM
Sample : 8330W-LOD1
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
HPLC_N
ClientSampleId :
8330W-LOD1


Manual Integrations
APPROVED

AHPatel
9/11/2012 5:08:08 AM

Integration File: events.e
Quant Time: Sep 07 02:29:12 2012
Quant Method : S:\HPCHEM1\HPLC_N\Method\HN081512.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Thu Aug 16 10:32:31 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

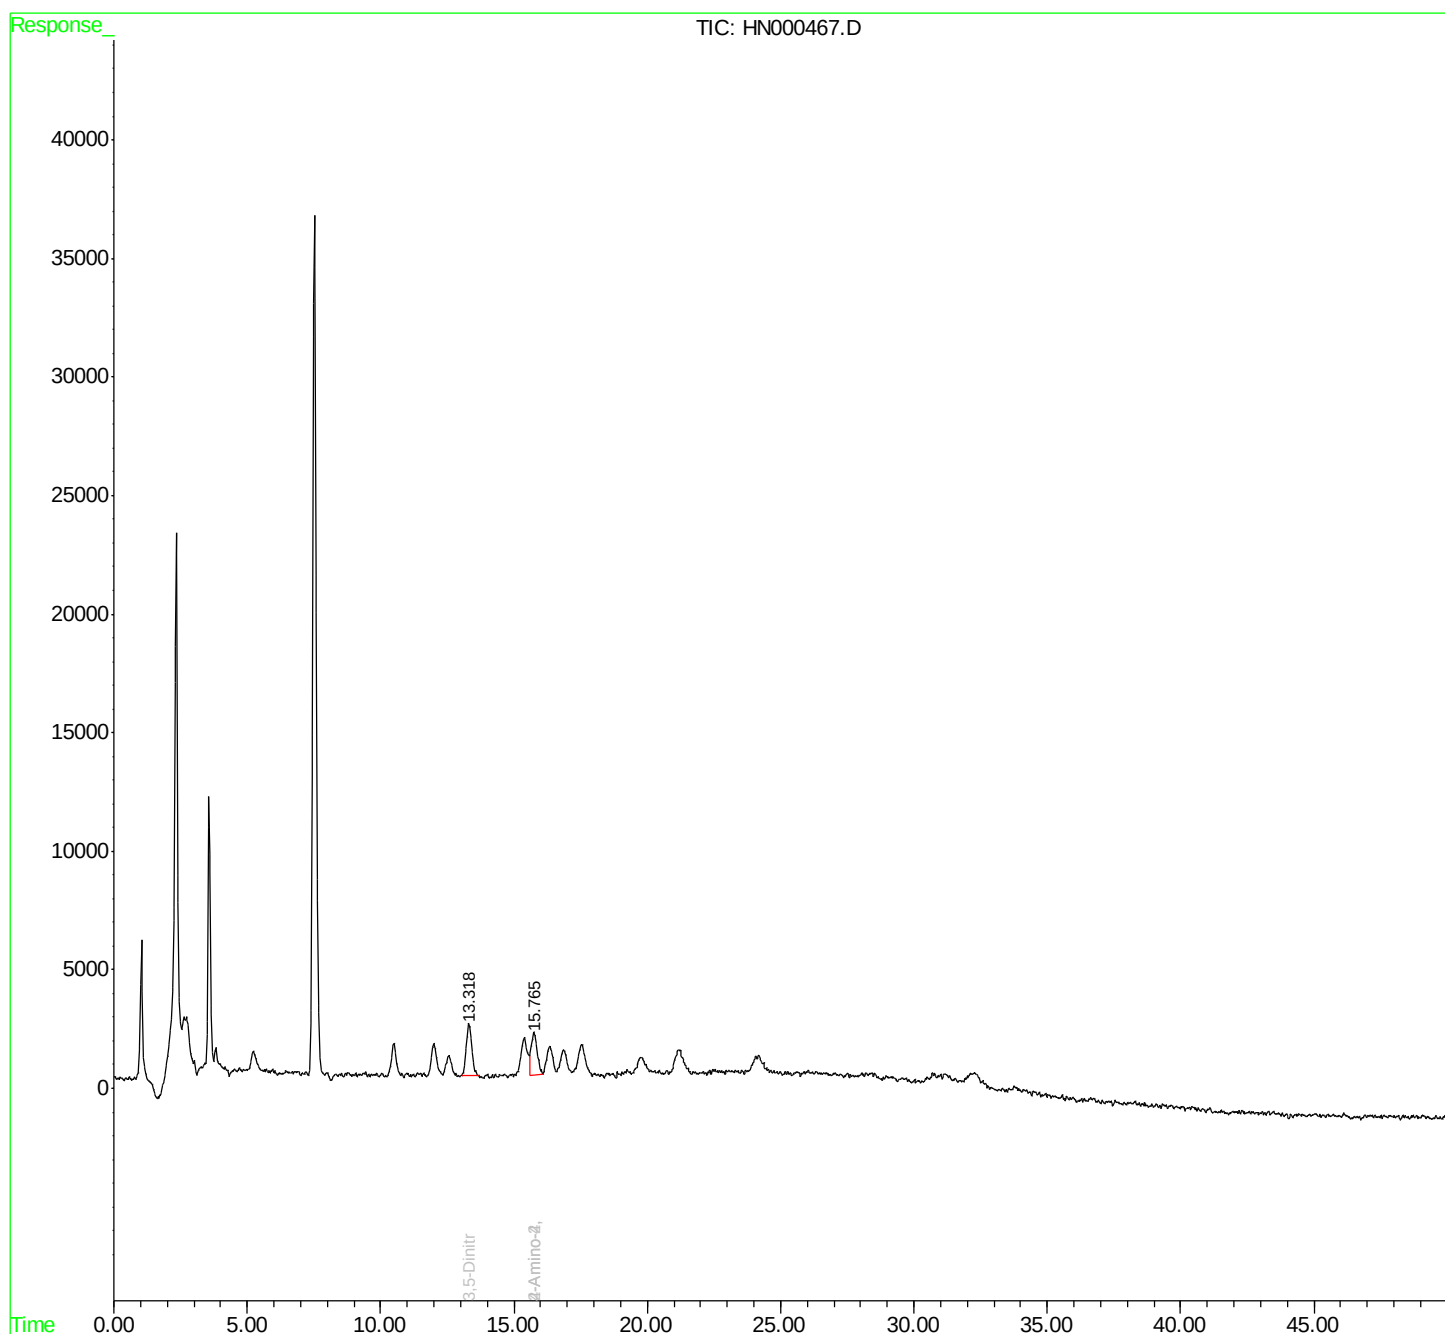

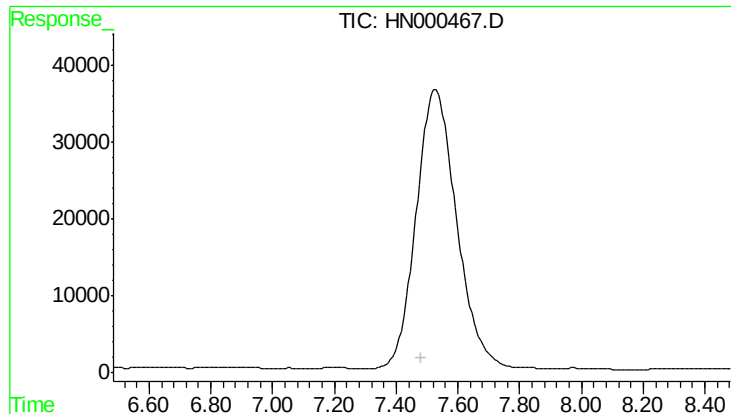


#1 4-Nitroaniline

R.T.: 0.000 min
 Exp R.T.: 7.483 min
 Response: 0
 Conc: N.D.

Instrument :
 HPLC_N
 ClientSampleId :
 8330W-LOD1


Manual Integrations
 APPROVED

AHPatel
 9/11/2012 5:08:08 AM

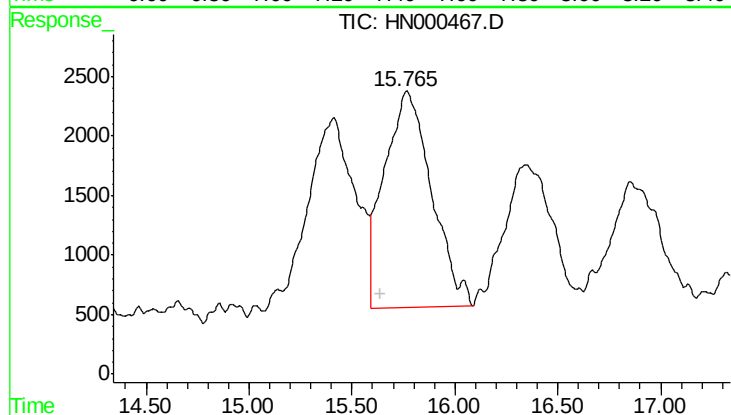


#7 2-Amino-4,6-dinitrotoluene

R.T.: 15.767 min
 Delta R.T.: 0.132 min
 Response: 292176
 Conc: 6.14 ug/L

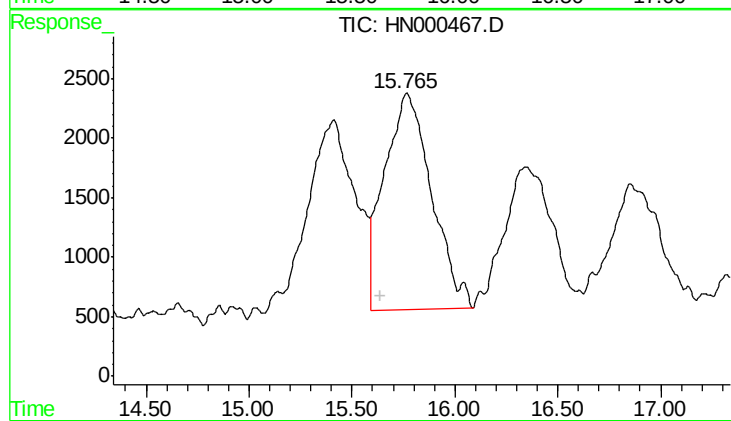

#8 4-Amino-2,6-dinitrotoluene

R.T.: 15.767 min
 Delta R.T.: 0.132 min
 Response: 292176
 Conc: 6.14 ug/L

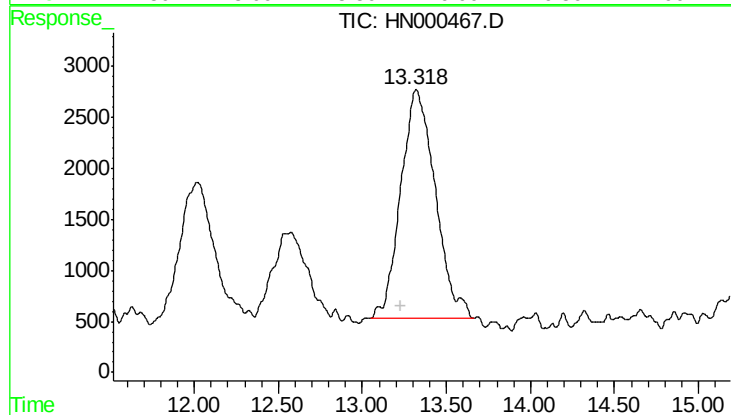

#16 3,5-Dinitroaniline

R.T.: 13.320 min
 Delta R.T.: 0.094 min
 Response: 321238
 Conc: 9.58 ug/L

Data Path : S:\HPCHEM1\HPLC_N\Data\HN090512\
Data File : HN000467.D
Signal(s) : VWD1A.CH
Acq On : 05-Sep-2012, 22:04
Operator : HLM
Sample : 8330W-LOD1
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
8330W-LOD1

Manual Integrations
APPROVED

AHPatel
9/11/2012 5:08:08 AM

Integration File: events.e
Quant Time: Sep 07 02:29:12 2012
Quant Method : S:\HPCHEM1\HPLC_N\Method\HN081512.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Thu Aug 16 10:32:31 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
7) T	2-Amino-4,6-dinitroto...	15.767f	292176	6.144 ug/L
8) T	4-Amino-2,6-dinitroto...	15.767f	292176	6.144 ug/L
16) T	3,5-Dinitroaniline	13.320f	321238	9.584 ug/L

(f)=RT Delta > 1/2 Window

(m)=manual int.