

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN092916\
 Data File : HN007760.D
 Signal(s) : vwd1A.ch
 Acq On : 29-Sep-2016, 17:02
 Operator : UM/MA
 Sample : PB93676BS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 30 07:25:10 2016
 Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN092716.M
 Quant Title :
 QLast Update : Tue Sep 27 16:13:17 2016
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.340	936235	234.481 ug/L
Target Compounds			
2) T HMX	0.902	2278037	522.137 ug/L
4) T 1,3,5-Trinitrobenzene	2.671f	5580161	519.004 ug/L
5) T 1,3-Dinitrobenzene	3.558f	8674803	516.523 ng/ml
6) T 3,5-Dinitroaniline	3.959f	6815983	507.917 ug/L
7) T Nitrobenzene	4.755f	4930431	505.362 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN092916\
Data File : HN007760.D
Signal(s) : vwd1A.ch
Acq On : 29-Sep-2016, 17:02
Operator : UM/MA
Sample : PB93676BS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 30 07:25:10 2016
Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN092716.M
Quant Title :
QLast Update : Tue Sep 27 16:13:17 2016
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

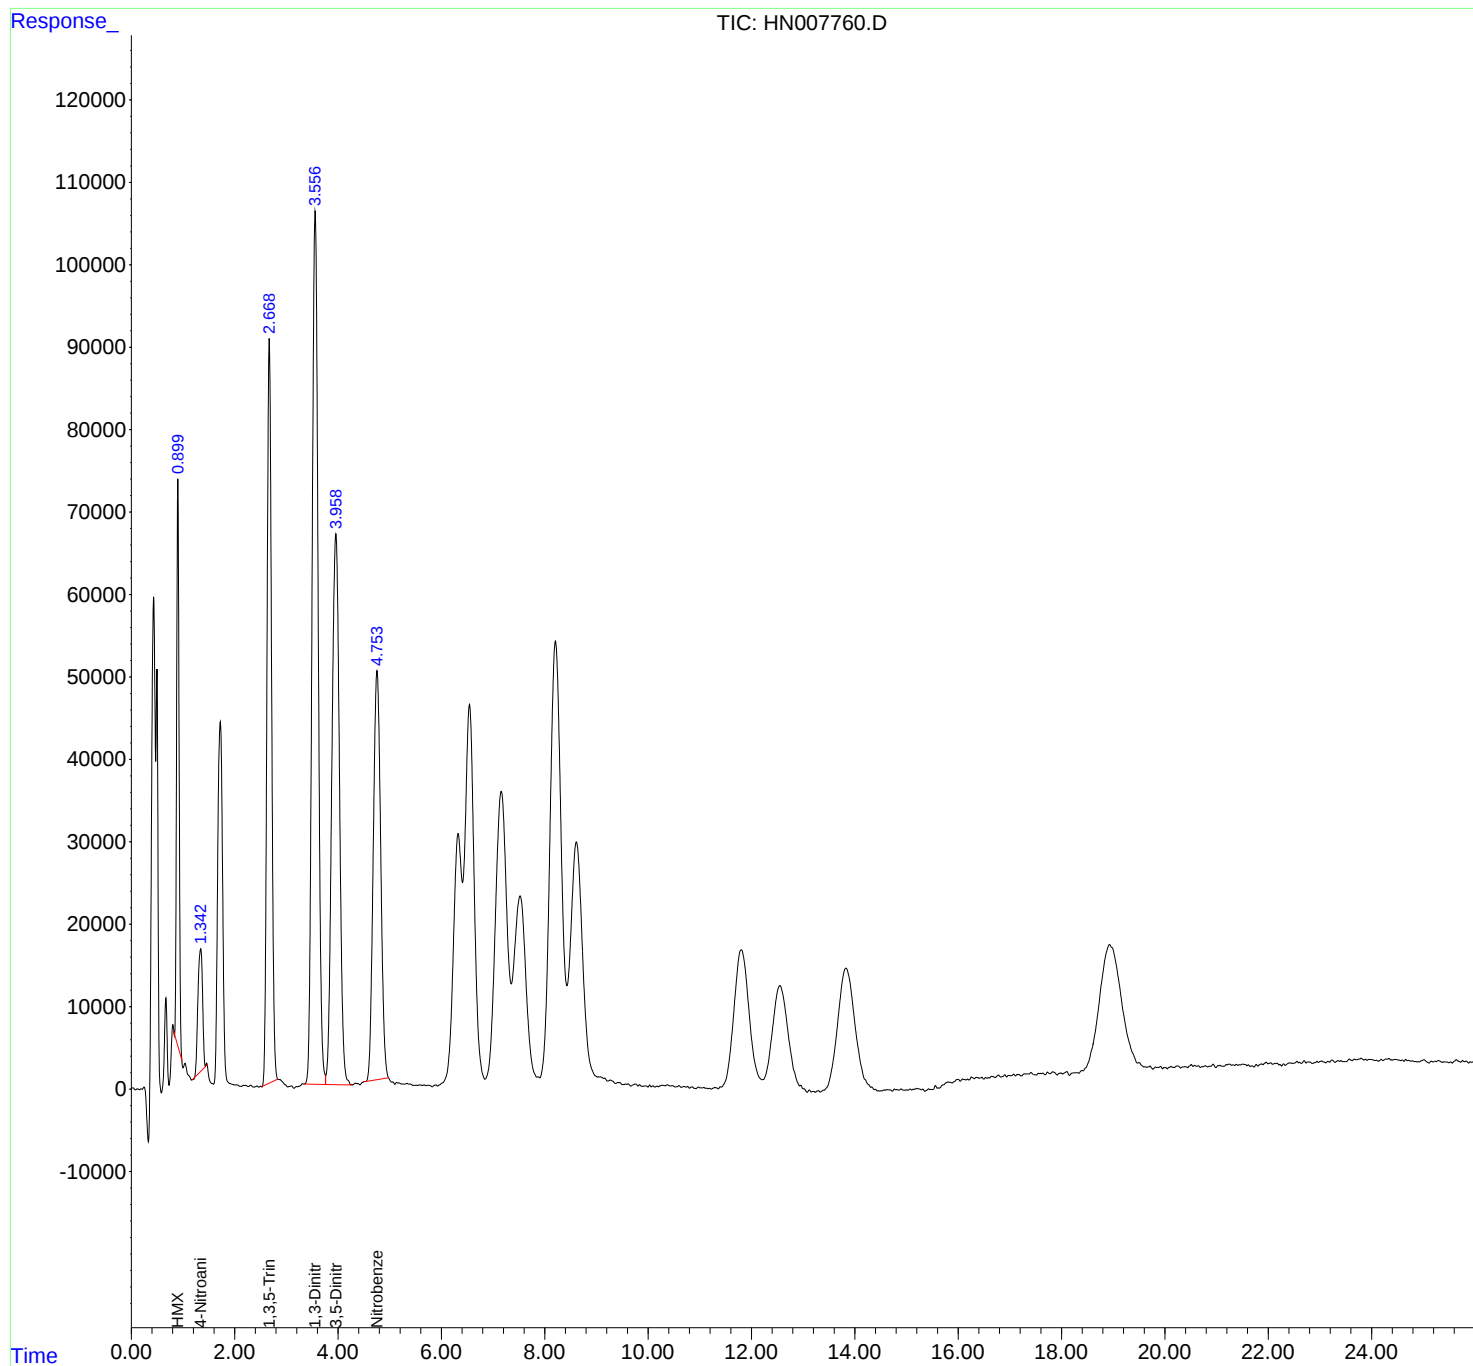


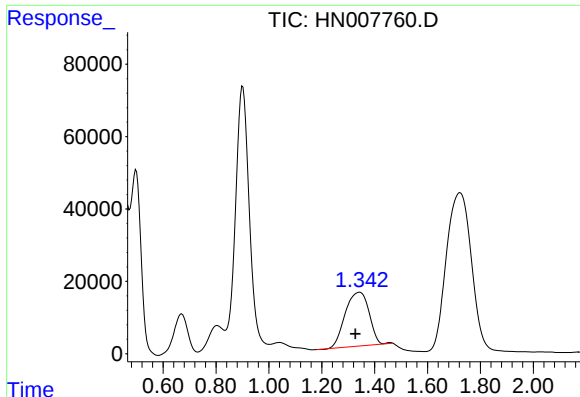

#1 4-Nitroaniline


R.T.: 1.340 min
Delta R.T.: 0.013 min
Response: 936235
Conc: 234.48 ug/L

Instrument :
HPLC_N
ClientSampleId :

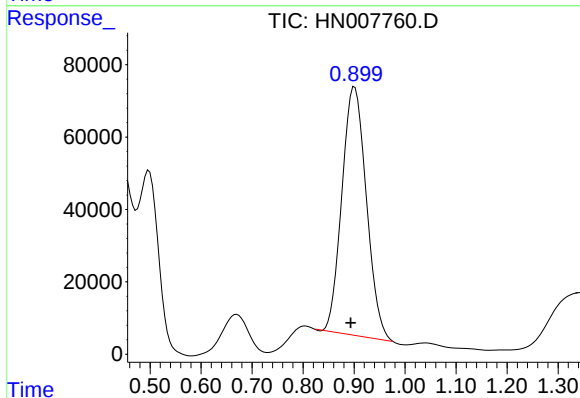


#2 HMX

R.T.: 0.902 min
Delta R.T.: 0.008 min
Response: 2278037
Conc: 522.14 ug/L

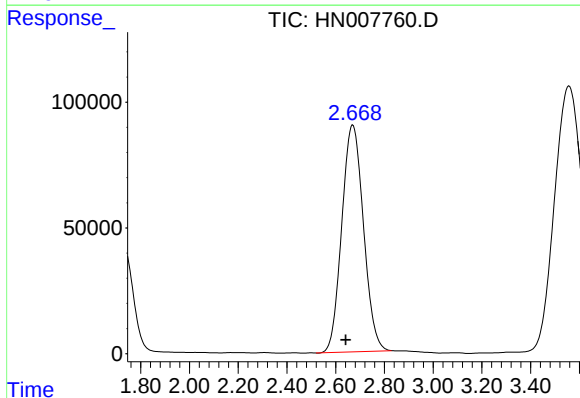


#4 1,3,5-Trinitrobenzene

R.T.: 2.671 min
Delta R.T.: 0.029 min
Response: 5580161
Conc: 519.00 ug/L

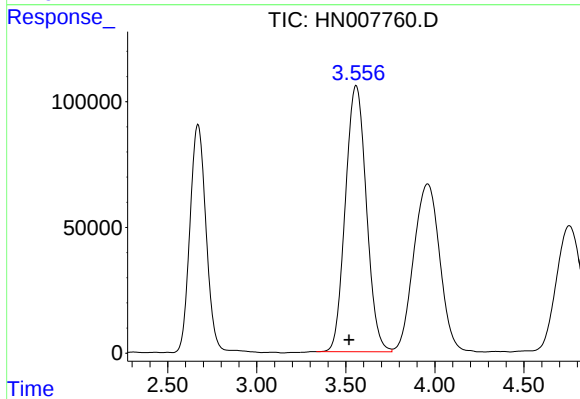

#5 1,3-Dinitrobenzene

R.T.: 3.558 min
Delta R.T.: 0.040 min
Response: 8674803
Conc: 516.52 ng/ml

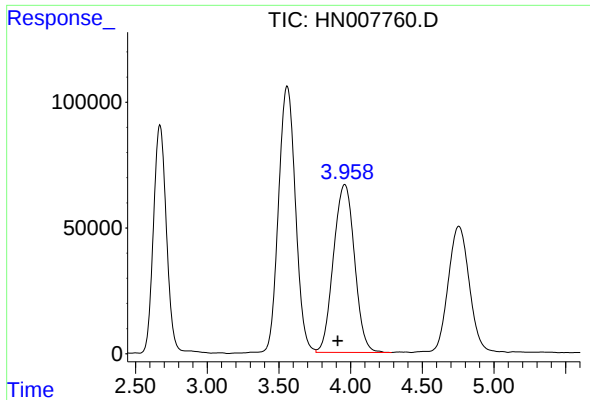

#6 3,5-Dinitroaniline


R.T.: 3.959 min

Delta R.T.: 0.047 min

Response: 6815983

Conc: 507.92 ug/L

Instrument :
HPLC_N
ClientSampleId :

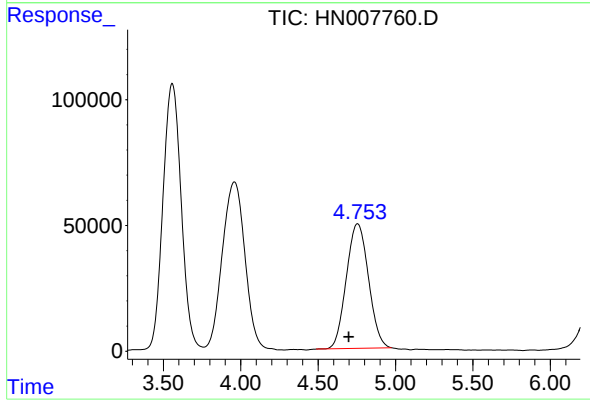

#7 Nitrobenzene

R.T.: 4.755 min

Delta R.T.: 0.057 min

Response: 4930431

Conc: 505.36 ug/L