

Signal #1 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006240.D\VWD1A.CH Vial: Instrument :
Signal #2 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006240.D\VWD1A.CH HPLC_N
Acq On : 30-Sep-2014, 11:22 Operator: HNP ClientSampleId :
Sample : HSTDICC5000 Inst : G1314A HSTDICC5000
Misc : Multiplr: 1.00
IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e
Quant Time: Oct 1 3:52 2014 Quant Results File: HN073114.RES

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN073114.M
Title :
Last Update : Thu Jul 31 18:00:41 2014
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

6) T	3,5-Dinitroaniline	6.48	44187650	2337.743 ug/L
------	--------------------	------	----------	---------------

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN006240.D HN073114.M

Thu Oct 09 13:55:20 2014



RPT1


Quantitation Report

Signal #1 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006240.D\VWD1A.CH Vial: Instrument :
Signal #2 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006240.D\VWD1A.CH HPLC_N
Acq On : 30-Sep-2014, 11:22 Operator: HNP ClientSampleId :
Sample : HSTDICC5000 Inst : G1314A HSTDICC5000
Misc : Multiplr: 1.00
IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e
Quant Time: Oct 1 3:52 2014 Quant Results File: HN073114.RES

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN073114.M
Title :
Last Update : Thu Jul 31 18:00:41 2014
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

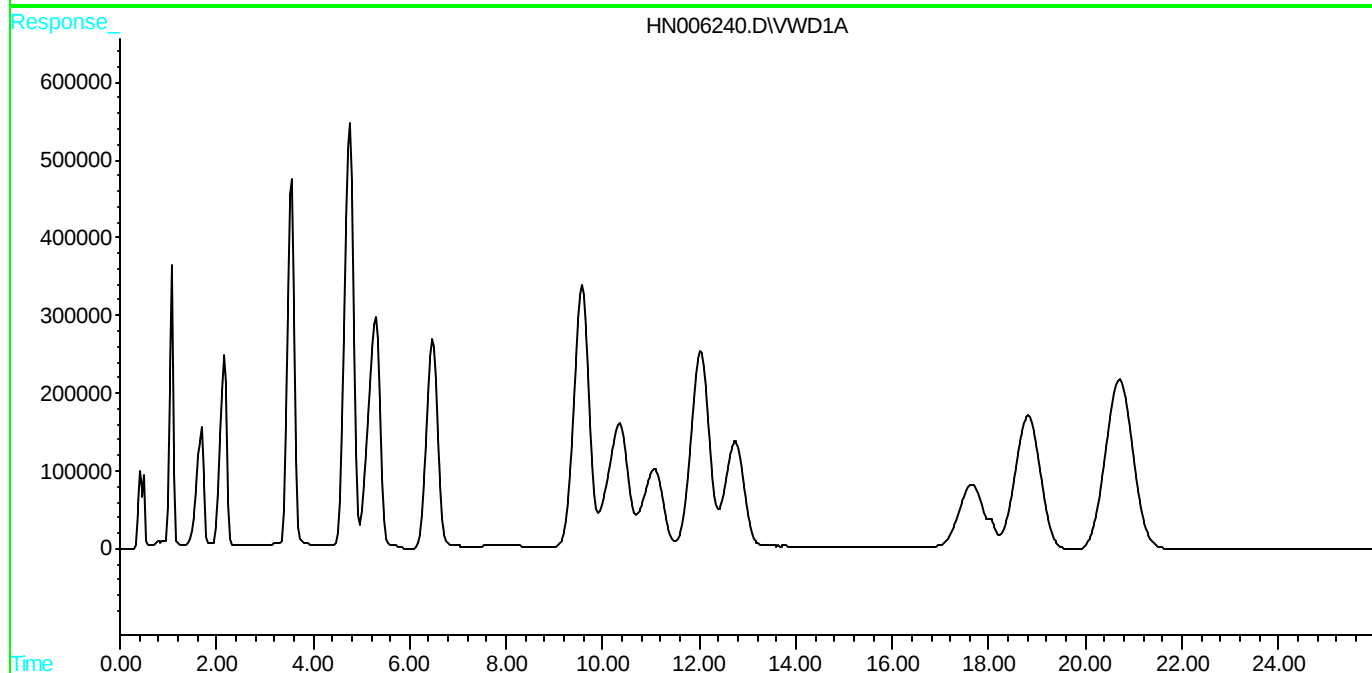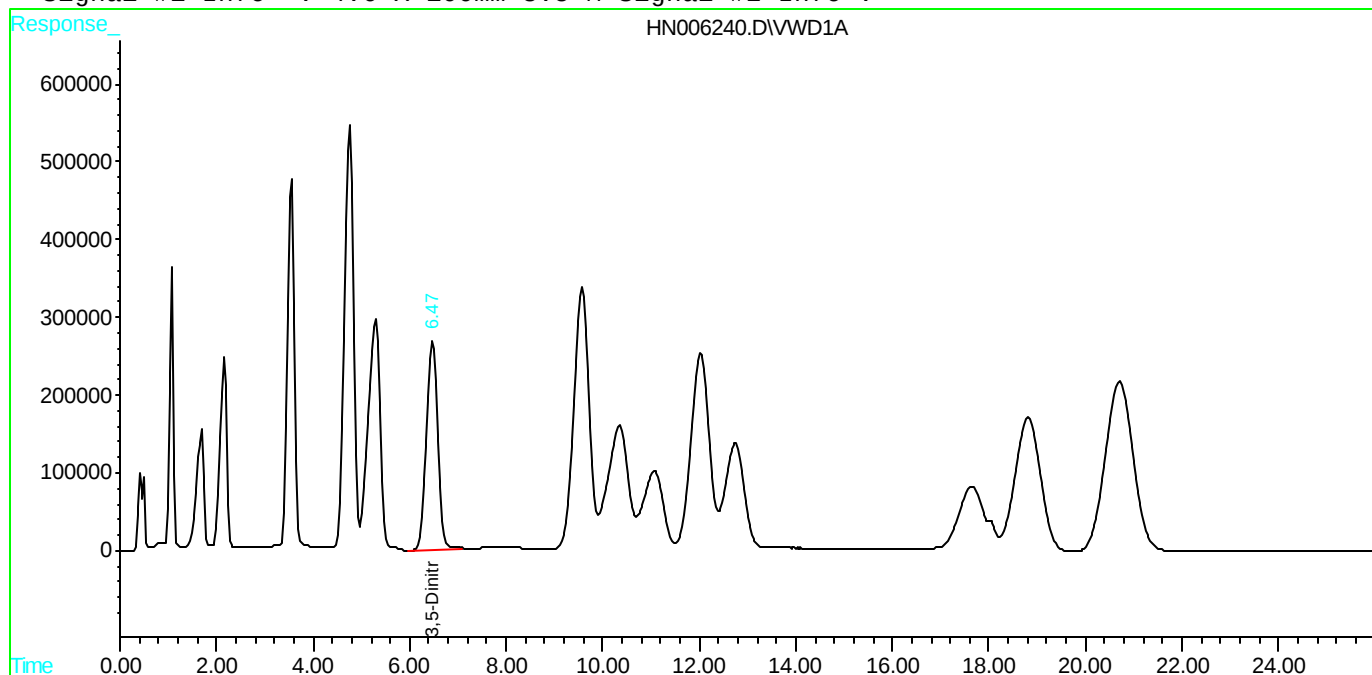


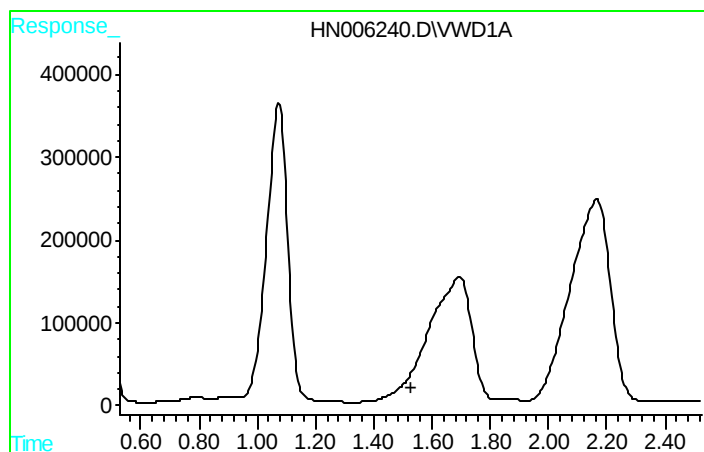

#1 4-Nitroaniline

R.T.: 0.000 min
 Exp R.T. : 1.529 min
 Response: 0
 Conc: N.D.

Instrument :
 HPLC_N
 ClientSampleId :
 HSTDICC5000

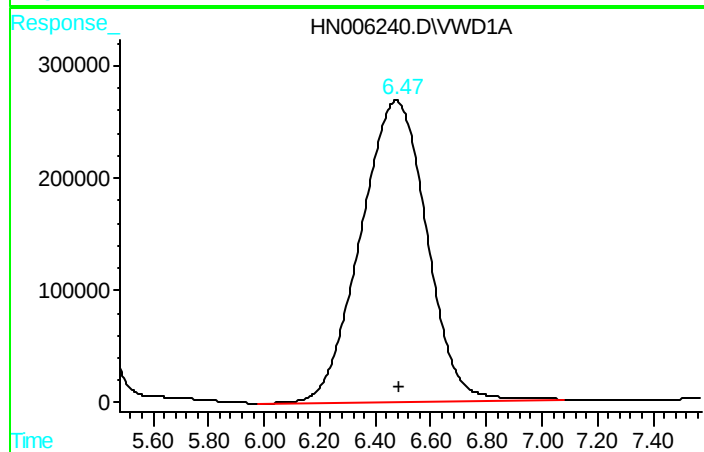

#6 3,5-Dinitroaniline

R.T.: 6.476 min
 Delta R.T.: -0.007 min
 Response: 44187650
 Conc: 2337.74 ug/L