

Signal #1 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006246.D\VWD1A.CH Vial: Instrument :
Signal #2 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006246.D\VWD1A.CH HPLC_N
Acq On : 30-Sep-2014, 14:10 Operator: HNP ClientSampleId :
Sample : PB79088BL Inst : G1314A PB79088BL
Misc : Multiplr: 1.00
IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e
Quant Time: Oct 1 5:56 2014 Quant Results File: HN093014.RES

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN093014.M
Title :
Last Update : Wed Oct 01 04:09:40 2014
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

2) T HMX	0.49	2334683	264.663 ug/L
----------	------	---------	--------------

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN006246.D HN093014.M Thu Oct 09 14:02:49 2014 RPT1



Quantitation Report


Signal #1 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006246.D\VWD1A.CH Vial:
Signal #2 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006246.D\VWD1A.CH
Acq On : 30-Sep-2014, 14:10 Operator: HNP
Sample : PB79088BL Inst : G1314A
Misc : Multiplr: 1.00
IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e
Quant Time: Oct 1 5:56 2014 Quant Results File: HN093014.RES

Instrument :
HPLC_N
ClientSampleId :
PB79088BL

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN093014.M
Title :
Last Update : Wed Oct 01 04:09:40 2014
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

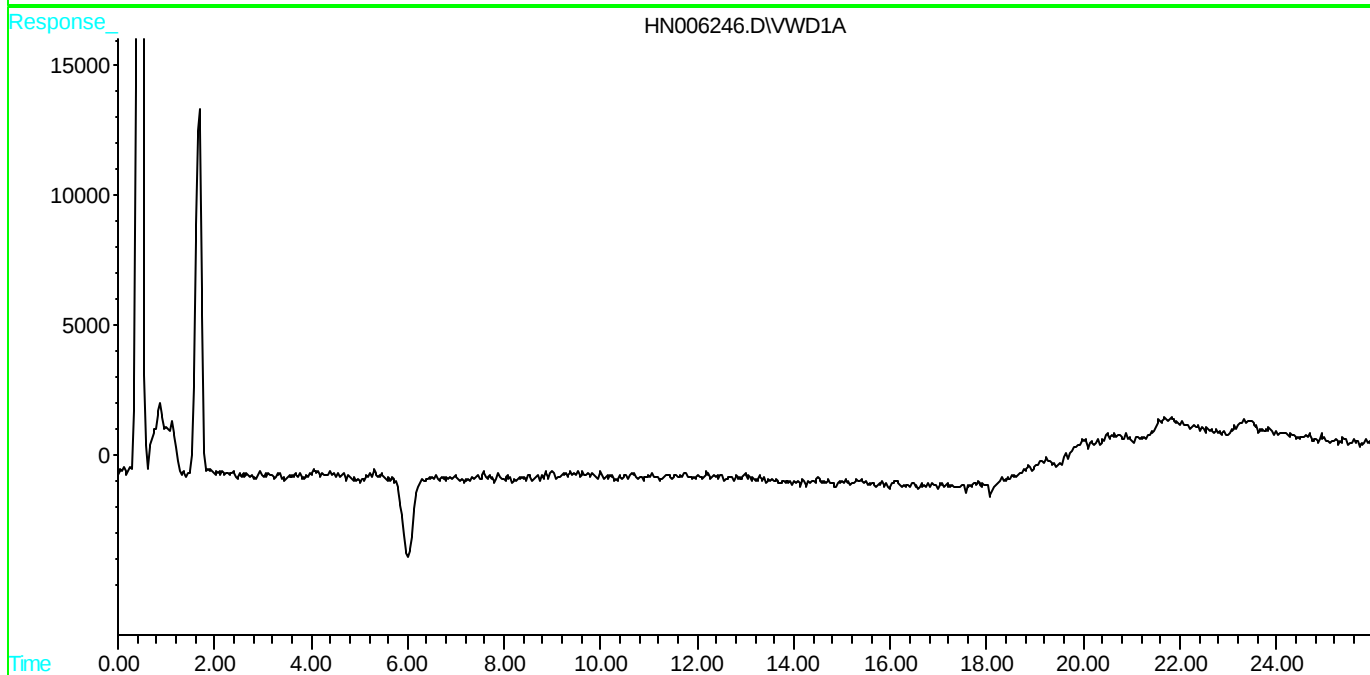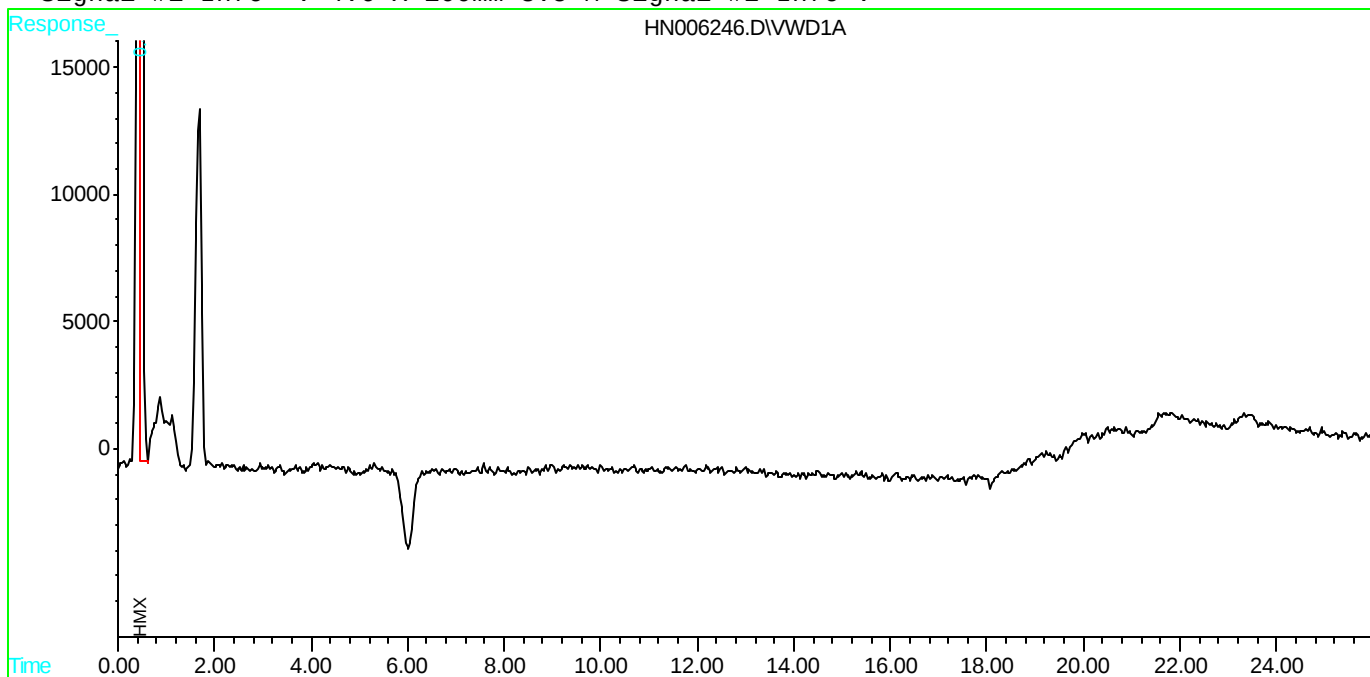


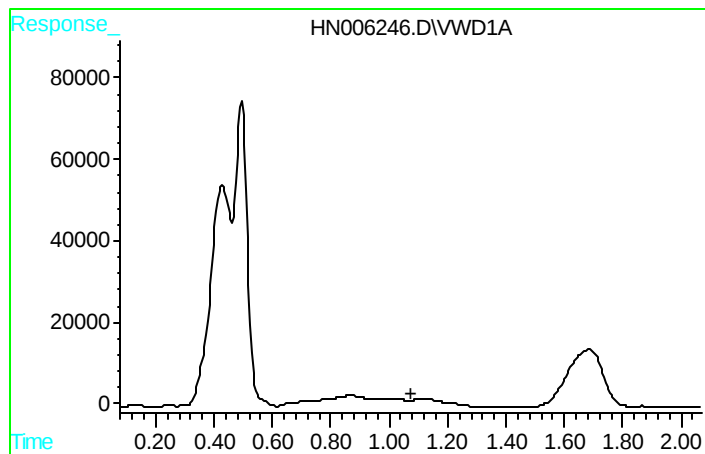

#1 4-Nitroaniline

R.T.: 0.000 min
Exp R.T.: 1.075 min
Response: 0
Conc: N.D.

Instrument :
HPLC_N
ClientSampleId :
PB79088BL

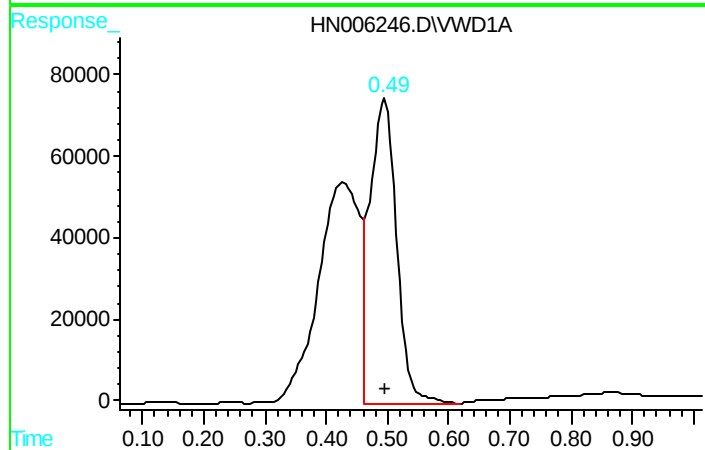

#2 HMX

R.T.: 0.495 min
Delta R.T.: 0.000 min
Response: 2334683
Conc: 264.66 ug/L