

Signal #1 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006251.D\VWD1A.CH Vial: Instrument :
Signal #2 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006251.D\VWD1A.CH HPLC_N
Acq On : 30-Sep-2014, 16:28 Operator: HNP LabSampleId :
Sample : HSTDICC020 Inst : G1314A HSTDICC020
Misc : Multiplr: 1.00
IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
Quant Time: Oct 1 4:38 2014 Quant Results File: HN0930NG.RES

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN0930NG.M
Title :
Last Update : Wed Oct 01 04:35:48 2014
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.69	77290650	20.146 ng/ul
Target Compounds			
2) T Nitroglycerin	8.27	149764292	20.087 ng/ul

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN006251.D HN0930NG.M

Thu Oct 09 14:06:57 2014



RPT1


Quantitation Report

Signal #1 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006251.D\VWD1A.CH Vial: Instrument :
Signal #2 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006251.D\VWD1A.CH HPLC_N
Acq On : 30-Sep-2014, 16:28 Operator: HNP LabSampleId :
Sample : HSTDICC020 Inst : G1314A HSTDICC020
Misc : Multiplr: 1.00
IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
Quant Time: Oct 1 4:38 2014 Quant Results File: HN0930NG.RES

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN0930NG.M
Title :
Last Update : Wed Oct 01 04:35:48 2014
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

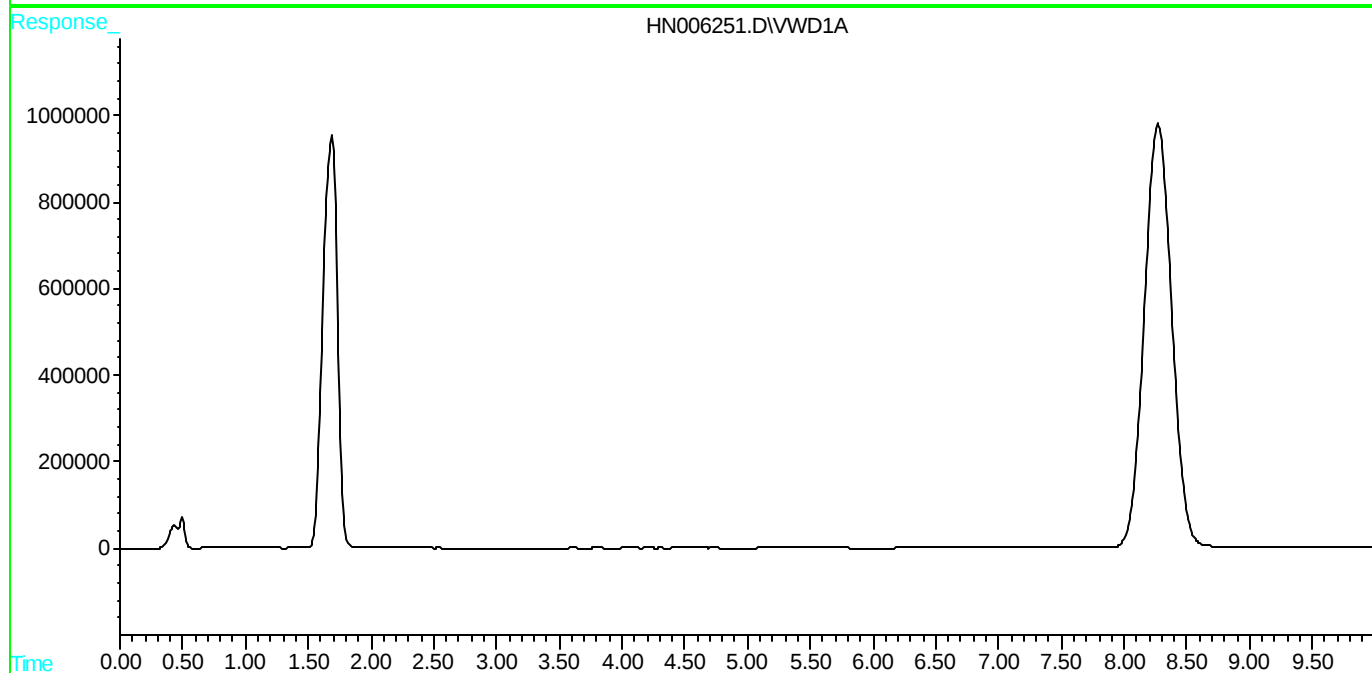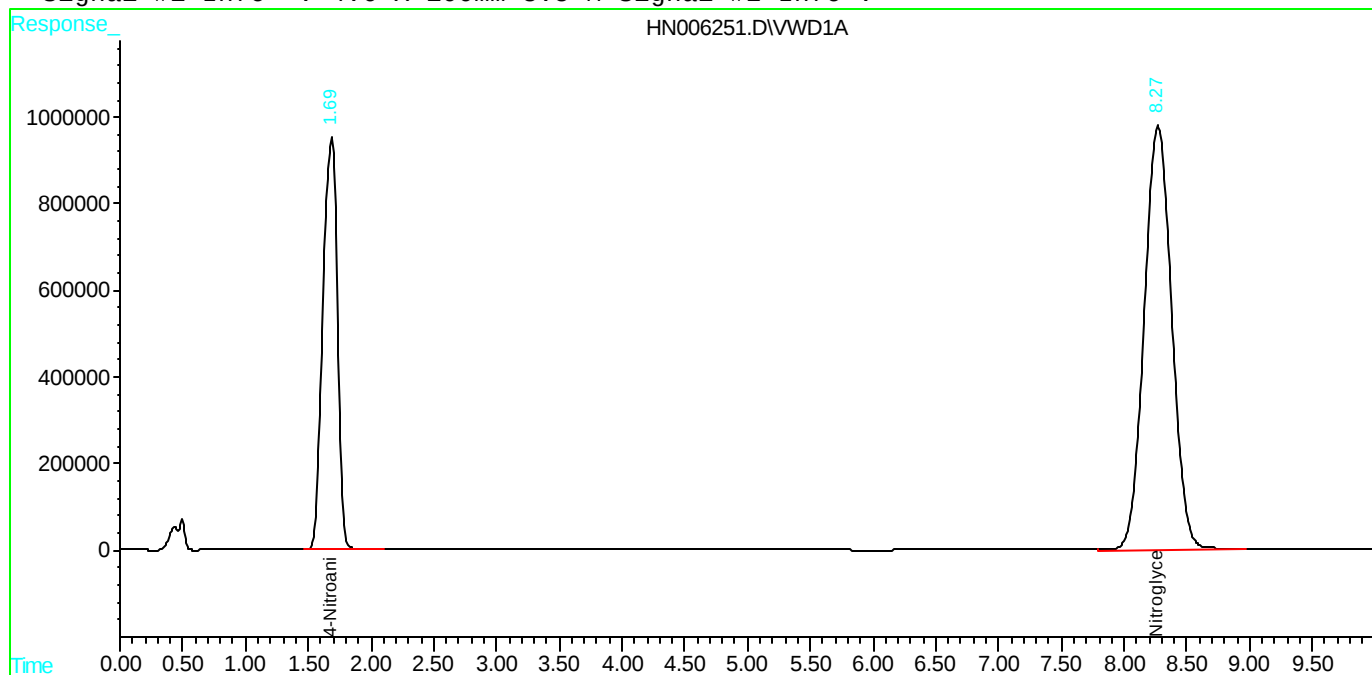


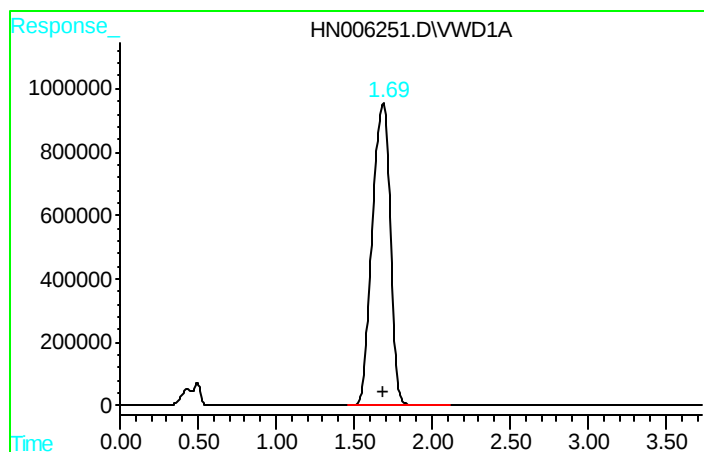

#1 4-Nitroaniline

R.T.: 1.689 min
 Delta R.T.: 0.000 min
 Response: 77290650
 Conc: 20.15 ng/ul

Instrument :
 HPLC_N
 LabSampleId :
 HSTDIC020

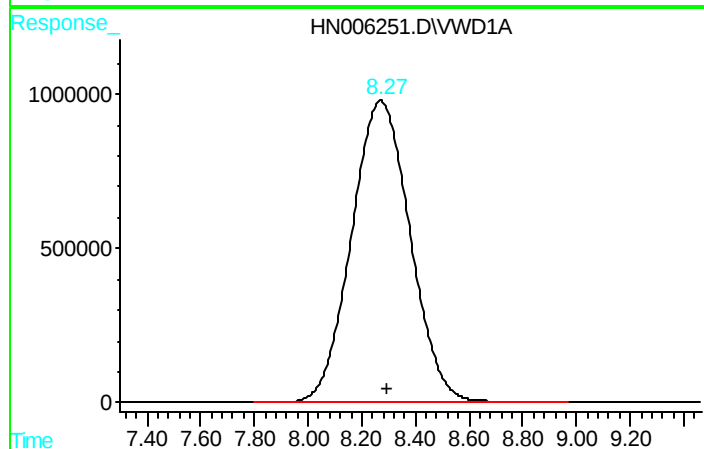

#2 Nitroglycerin

R.T.: 8.271 min
 Delta R.T.: -0.024 min
 Response: 149764292
 Conc: 20.09 ng/ul