

Signal #1 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006253.D\VWD1A.CH Vial: Instrument :
Signal #2 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006253.D\VWD1A.CH HPLC_N
Acq On : 30-Sep-2014, 16:52 Operator: HNP LabSampleId :
Sample : HSTDICCC005 Inst : G1314A HSTDICCC005
Misc : Multiplr: 1.00
IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
Quant Time: Oct 1 4:34 2014 Quant Results File: HN0930NG.RES

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN0930NG.M
Title :
Last Update : Tue Jan 21 14:02:23 2014
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.69	19410892	5.059 ng/ul
Target Compounds			
2) T Nitroglycerin	8.30	38125934	5.114 ng/ul

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN006253.D HN0930NG.M

Thu Oct 09 14:08:19 2014



RPT1


Quantitation Report

Signal #1 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006253.D\VWD1A.CH Vial: Instrument :
Signal #2 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006253.D\VWD1A.CH HPLC_N
Acq On : 30-Sep-2014, 16:52 Operator: HNP LabSampleId :
Sample : HSTDICCC005 Inst : G1314A HSTDICCC005
Misc : Multiplr: 1.00
IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
Quant Time: Oct 1 4:34 2014 Quant Results File: HN0930NG.RES

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN0930NG.M
Title :
Last Update : Tue Jan 21 14:02:23 2014
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

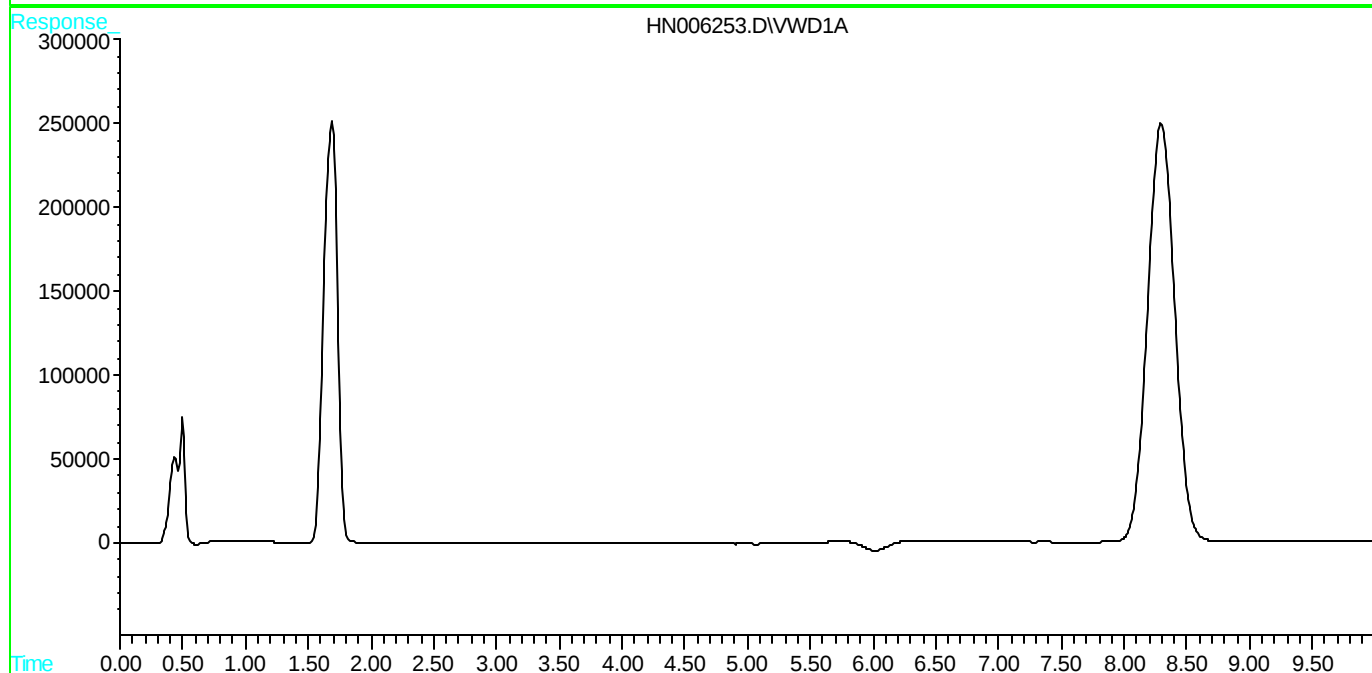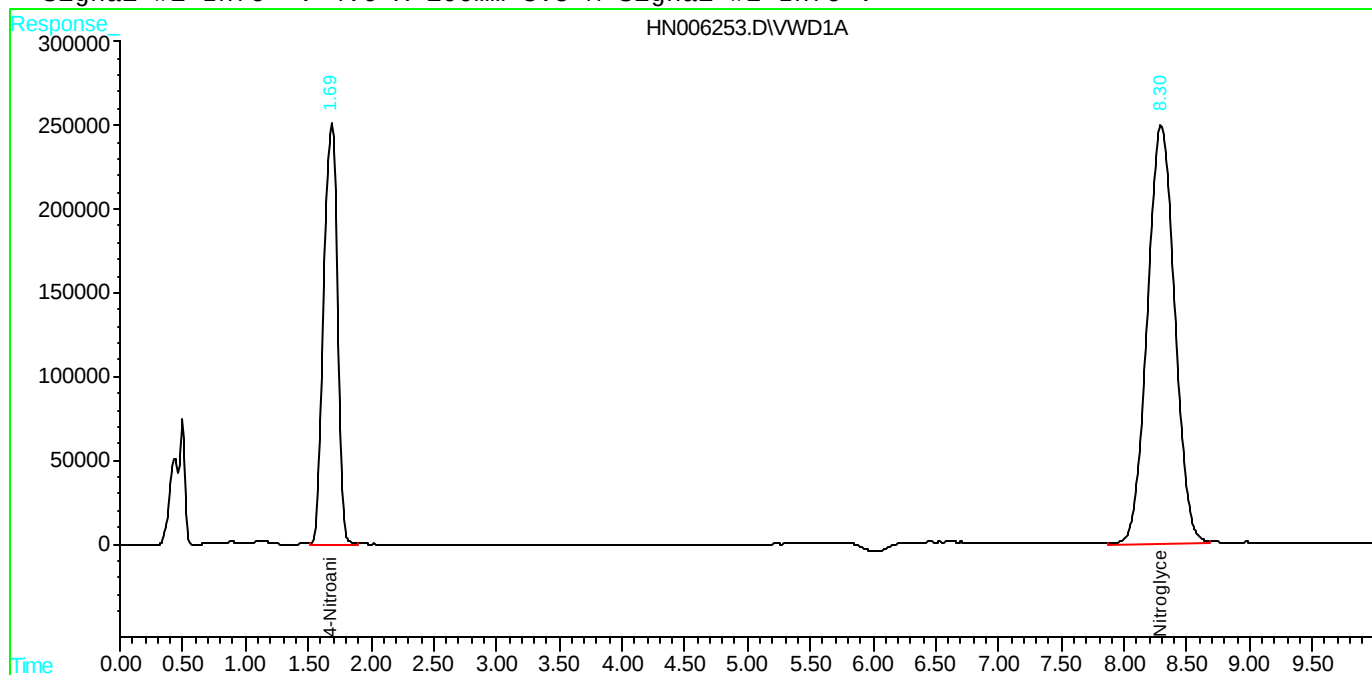


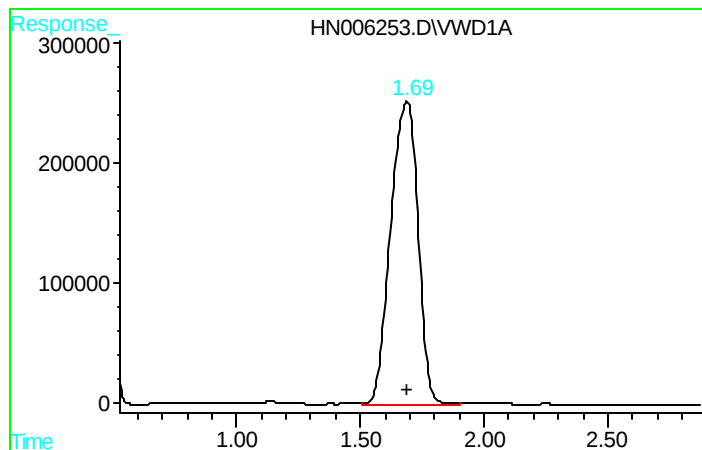

#1 4-Nitroaniline

R.T.: 1.690 min
 Delta R.T.: 0.002 min
 Response: 19410892
 Conc: 5.06 ng/ul

Instrument :
 HPLC_N
 LabSampleId :
 HSTDICCC005

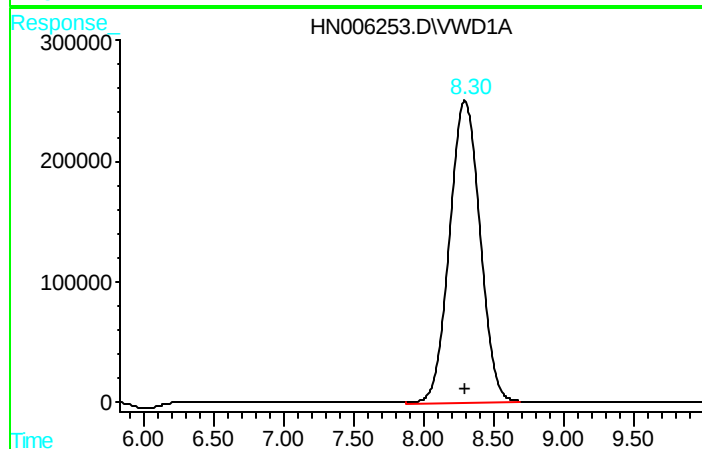

#2 Nitroglycerin

R.T.: 8.297 min
 Delta R.T.: 0.002 min
 Response: 38125934
 Conc: 5.11 ng/ul