

Signal #1 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006255.D\VWD1A.CH Vial:
Signal #2 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006255.D\VWD1A.CH
Acq On : 30-Sep-2014, 17:16 Operator: HNP
Sample : HSTDICC0.5 Inst : G1314A
Misc : Multiplr: 1.00
IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
Quant Time: Oct 1 4:42 2014 Quant Results File: HN0930NG.RES

Instrument :
HPLC_N
LabSampleId :
HSTDICC0.5

Manual Integrations
APPROVED

mohammad
10/9/2014 2:25:39 PM

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN0930NG.M
Title :
Last Update : Wed Oct 01 04:35:48 2014
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.69	1986894	0.518 ng/ul
Target Compounds			
2) T Nitroglycerin	8.29	3639875	0.488 ng/ulm

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN006255.D HN0930NG.M

Thu Oct 09 14:09:46 2014

RPT1

Quantitation Report

Signal #1 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006255.D\VWD1A.CH Vial:
Signal #2 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006255.D\VWD1A.CH
Acq On : 30-Sep-2014, 17:16 Operator: HNP
Sample : HSTDICC0.5 Inst : G1314A
Misc : Multiplr: 1.00
IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
Quant Time: Oct 1 4:42 2014 Quant Results File: HN0930NG.RES



Instrument :
HPLC_N
LabSampleId :
HSTDICC0.5


Manual Integrations
APPROVED

mohammad
10/9/2014 2:25:39 PM

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN0930NG.M
Title :
Last Update : Wed Oct 01 04:35:48 2014
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

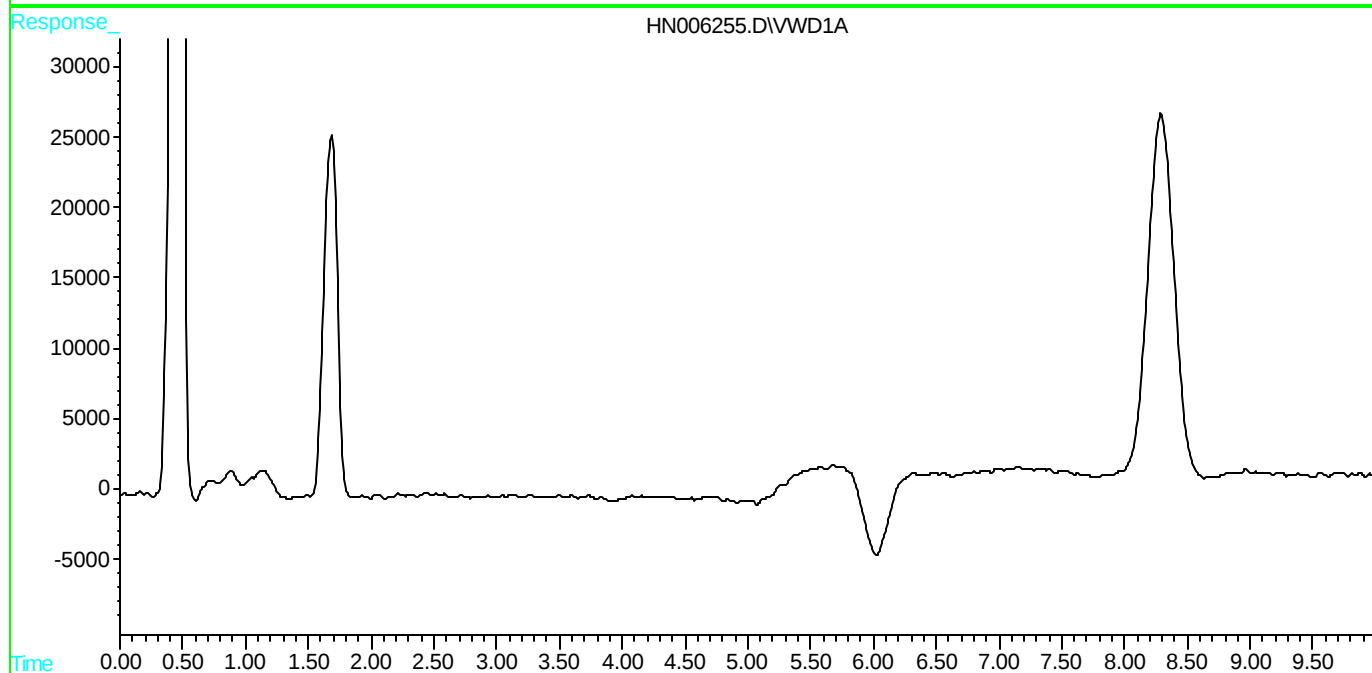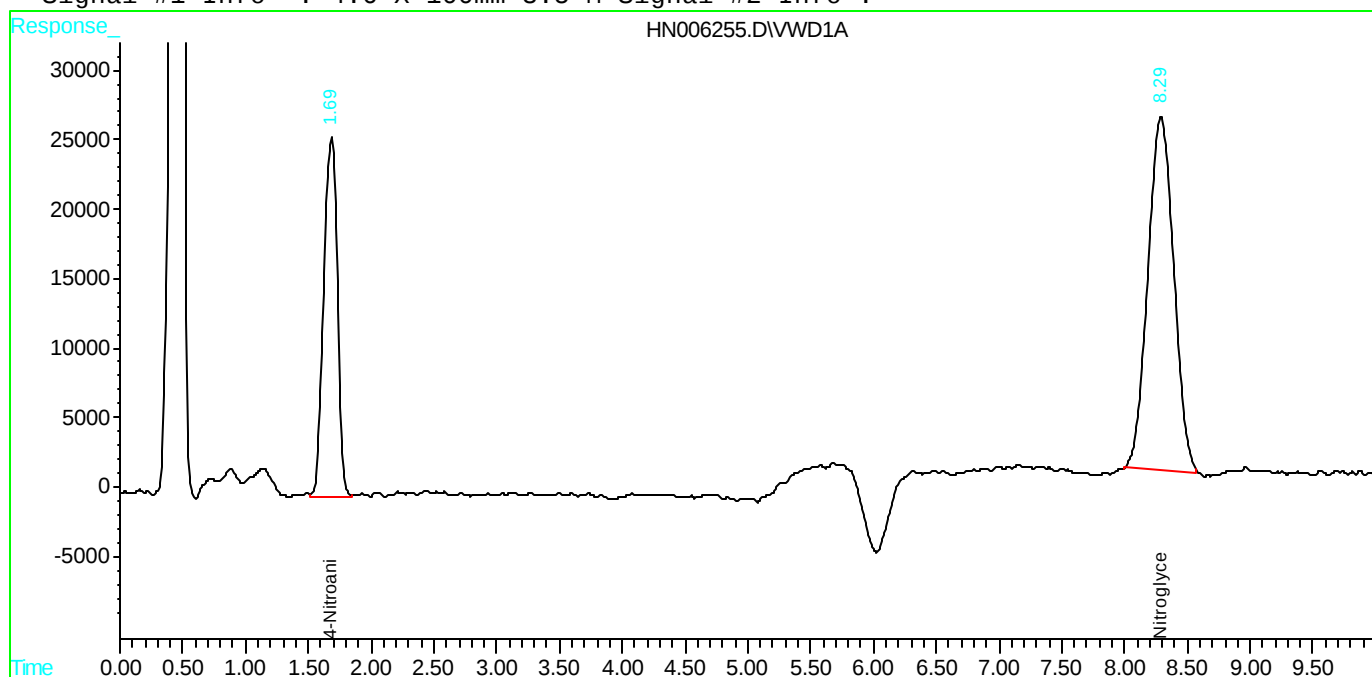

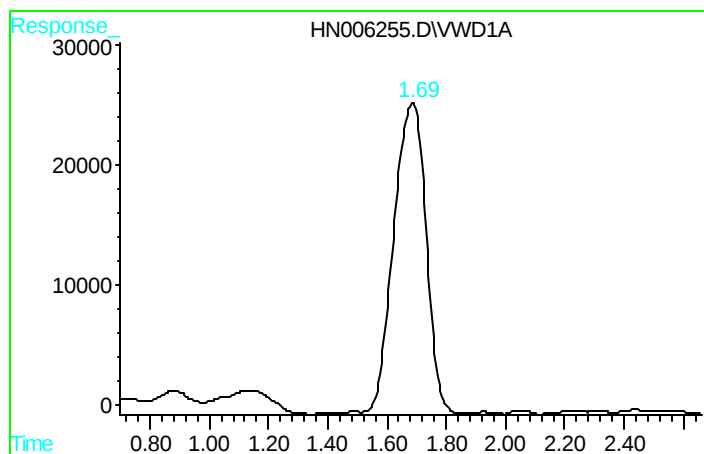


#1 4-Nitroaniline

R.T.: 1.688 min
 Delta R.T.: 0.000 min
 Response: 1986894
 Conc: 0.52 ng/ul

Instrument :
 HPLC_N
 LabSampleId :
 HSTDIC0.5

Manual Integrations
 APPROVED

mohammad
 10/9/2014 2:25:39 PM

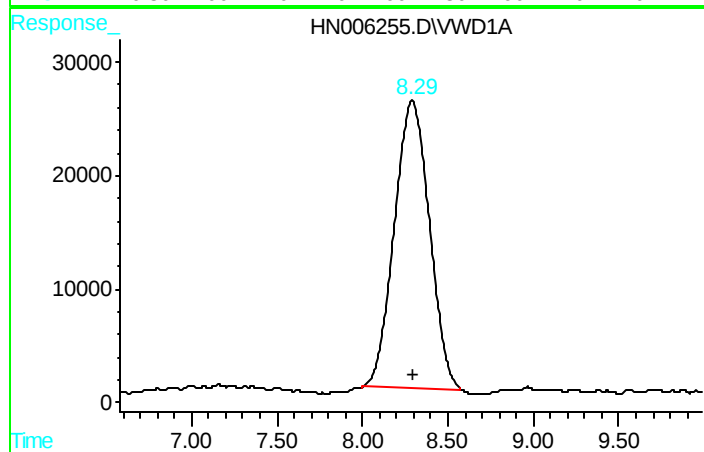

#2 Nitroglycerin

R.T.: 8.289 min
 Delta R.T.: -0.007 min
 Response: 3639875
 Conc: 0.49 ng/ul m