

Signal #1 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006259.D\VWD1A.CH Vial: Instrument :
Signal #2 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006259.D\VWD1A.CH HPLC_N
Acq On : 30-Sep-2014, 18:04 Operator: HNP ClientSampleId :
Sample : F3897-21 Inst : G1314A RR-EXP-WP
Misc : Multiplr: 1.00
IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
Quant Time: Oct 1 4:50 2014 Quant Results File: HN0930NG.RES

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN0930NG.M
Title :
Last Update : Wed Oct 01 04:43:51 2014
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.68	1204975	0.306 ng/ul

Target Compounds

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN006259.D HN0930NG.M

Thu Oct 09 14:16:49 2014



RPT1


Quantitation Report

Signal #1 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006259.D\VWD1A.CH Vial: Instrument :
Signal #2 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006259.D\VWD1A.CH HPLC_N
Acq On : 30-Sep-2014, 18:04 Operator: HNP ClientSampleId :
Sample : F3897-21 Inst : G1314A RR-EXP-WP
Misc : Multiplr: 1.00
IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
Quant Time: Oct 1 4:50 2014 Quant Results File: HN0930NG.RES

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN0930NG.M
Title :
Last Update : Wed Oct 01 04:43:51 2014
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

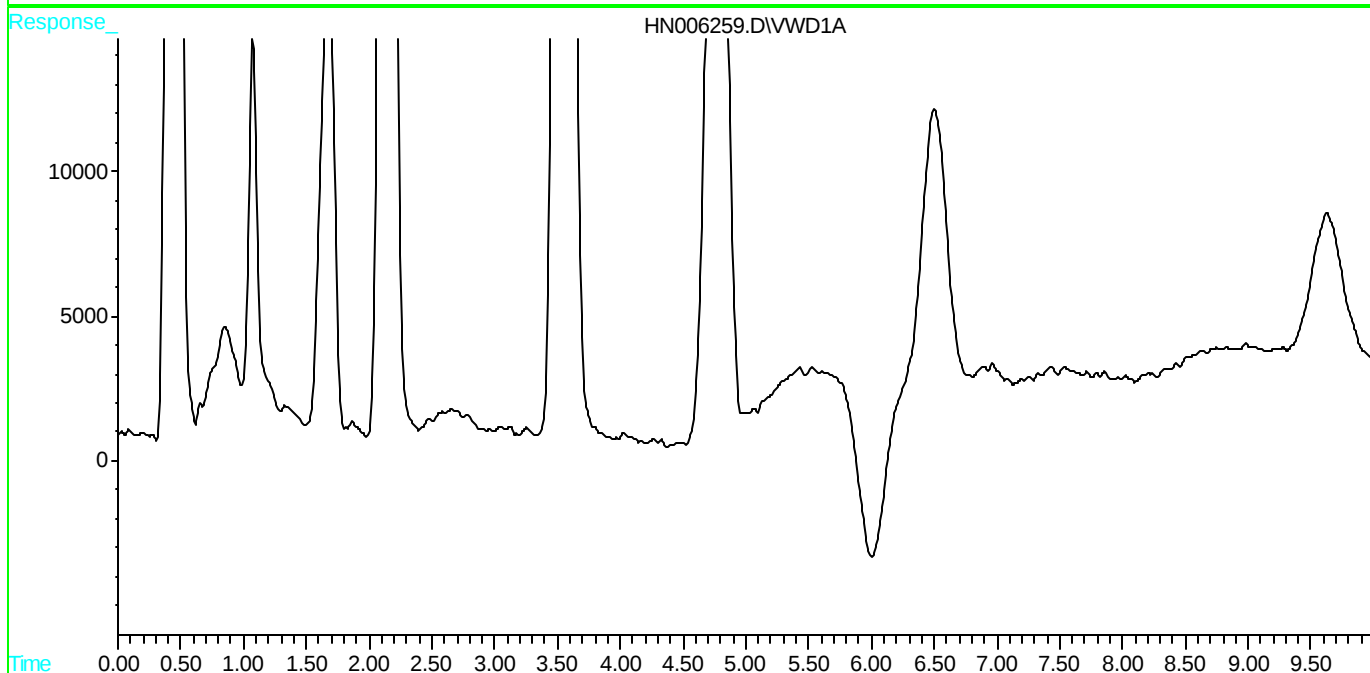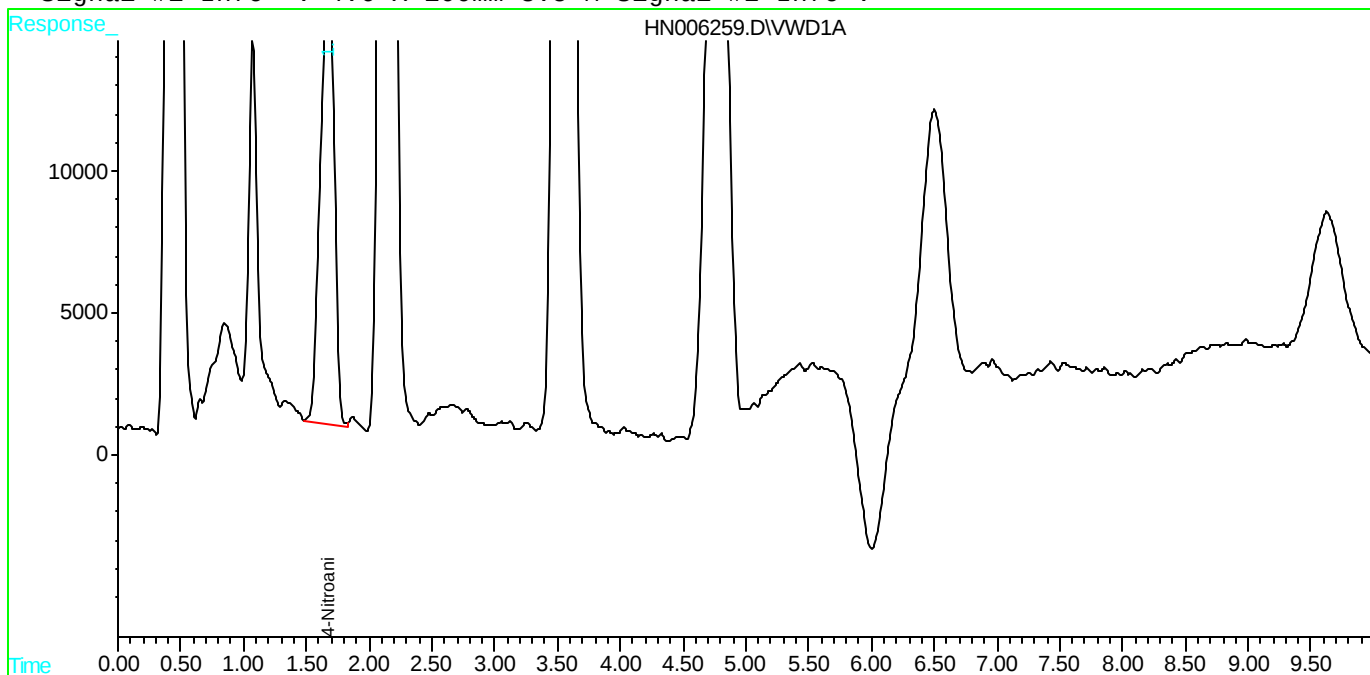

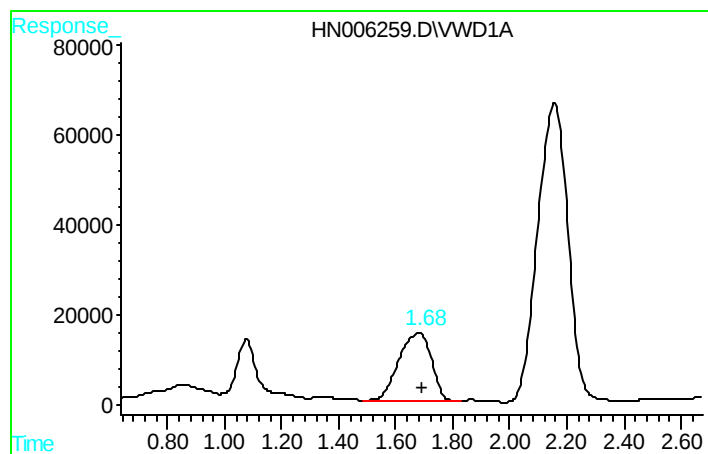

#1 4-Nitroaniline

R.T.: 1.684 min
Delta R.T.: -0.006 min
Response: 1204975
Conc: 0.31 ng/ul

Instrument :
HPLC_N
ClientSampleId :
RR-EXP-WP