

Signal #1 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006260.D\VWD1A.CH Vial: Instrument :
Signal #2 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006260.D\VWD1A.CH HPLC_N
Acq On : 30-Sep-2014, 18:16 Operator: HNP LabSampleId :
Sample : HSTDCCC005 Inst : G1314A HSTDCCC005
Misc : Multiplr: 1.00
IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
Quant Time: Oct 1 4:52 2014 Quant Results File: HN0930NG.RES

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN0930NG.M
Title :
Last Update : Wed Oct 01 04:43:51 2014
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.70	19470790	4.948 ng/ul
Target Compounds			
2) T Nitroglycerin	8.33	39649749	5.272 ng/ul

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN006260.D HN0930NG.M

Thu Oct 09 14:17:33 2014



RPT1


Quantitation Report

Signal #1 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006260.D\VWD1A.CH Vial: Instrument :
Signal #2 : S:\HPCHEM1\HPLC_N\DATA\HN093014\HN006260.D\VWD1A.CH HPLC_N
Acq On : 30-Sep-2014, 18:16 Operator: HNP LabSampleId :
Sample : HSTDCCC005 Inst : G1314A HSTDCCC005
Misc : Multiplr: 1.00
IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
Quant Time: Oct 1 4:52 2014 Quant Results File: HN0930NG.RES

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN0930NG.M
Title :
Last Update : Wed Oct 01 04:43:51 2014
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

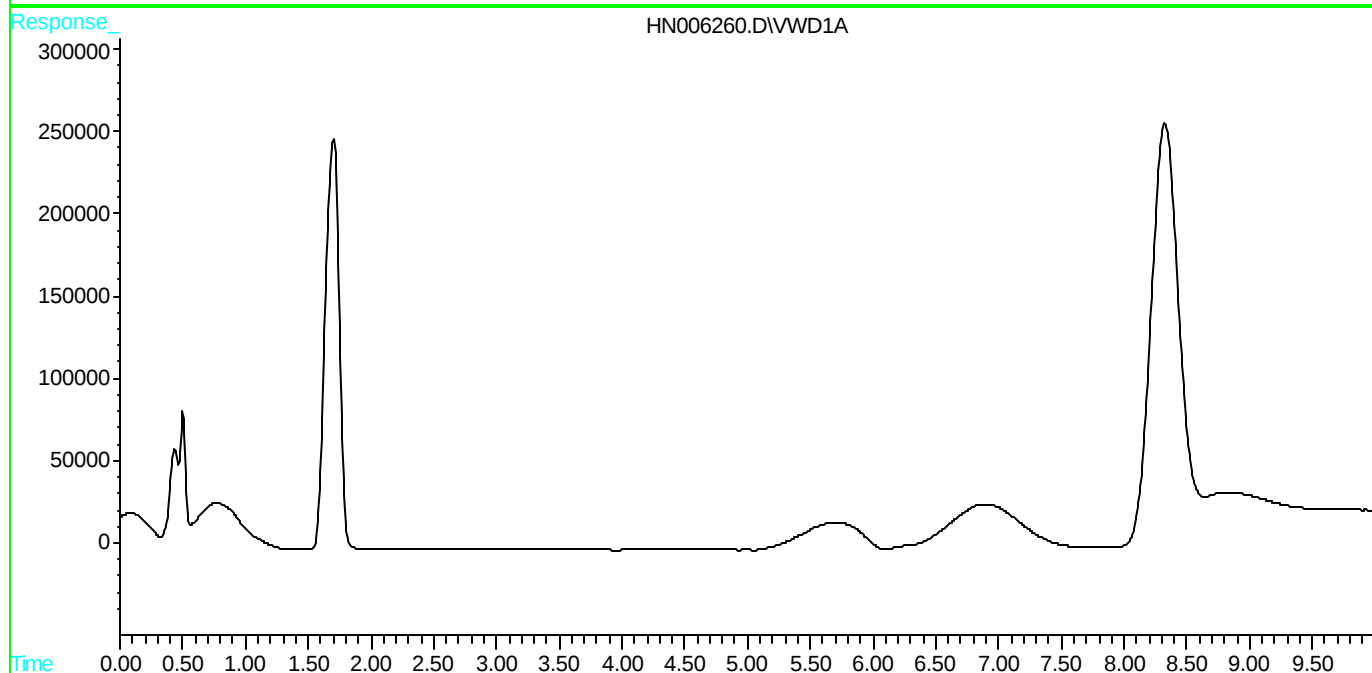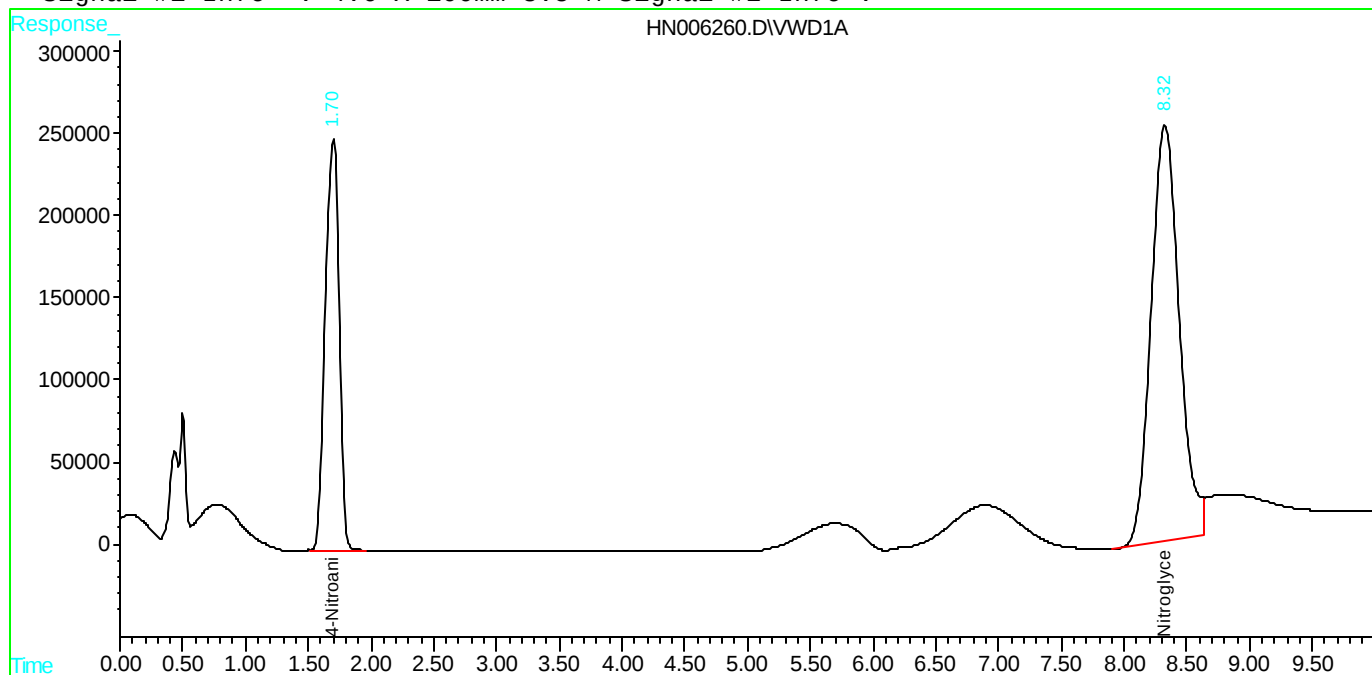


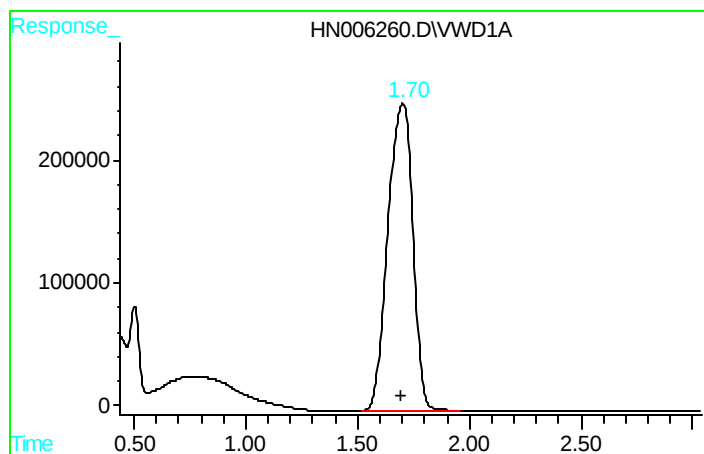

#1 4-Nitroaniline

R.T.: 1.704 min
Delta R.T.: 0.014 min
Response: 19470790
Conc: 4.95 ng/ul

Instrument :
HPLC_N
LabSampleId :
HSTDCCC005

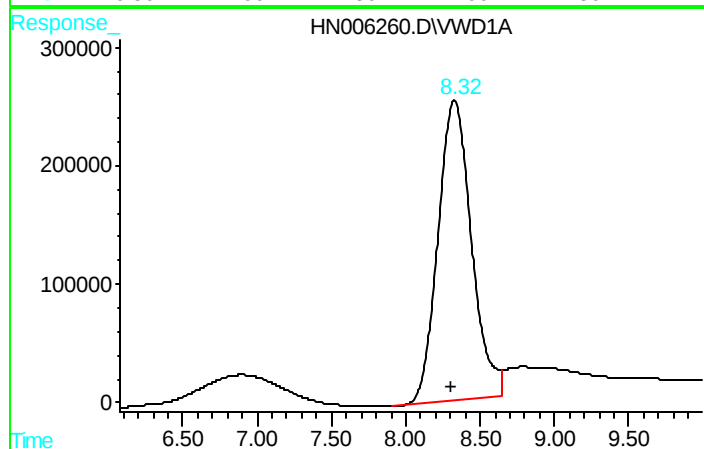

#2 Nitroglycerin

R.T.: 8.326 min
Delta R.T.: 0.029 min
Response: 39649749
Conc: 5.27 ng/ul