

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN100214\
 Data File : HN006265.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 02-Oct-2014, 10:17
 Operator : HNP
 Sample : HSTDICC5000
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 HSTDICC5000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 16:16:16 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
 Quant Title :
 QLast Update : Mon Mar 09 14:56:25 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.331	15013348	4406.363 ug/L
Target Compounds			
2) T HMX	0.881	22002289	4880.747 ug/L
3) T RDX	1.722	24822684	4734.516 ug/L
4) T 1,3,5-Trinitrobenzene	2.701	54578471	5083.910 ug/L
5) T 1,3-Dinitrobenzene	3.601	83542118	5120.691 ng/ml
6) T 3,5-Dinitroaniline	3.985f	57844579	4975.098 ug/L
7) T Nitrobenzene	4.870f	50637077	5028.155 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN100214\
Data File : HN006265.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 02-Oct-2014, 10:17
Operator : HNP
Sample : HSTDICC5000
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDICC5000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 16:16:16 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
Quant Title :
QLast Update : Mon Mar 09 14:56:25 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

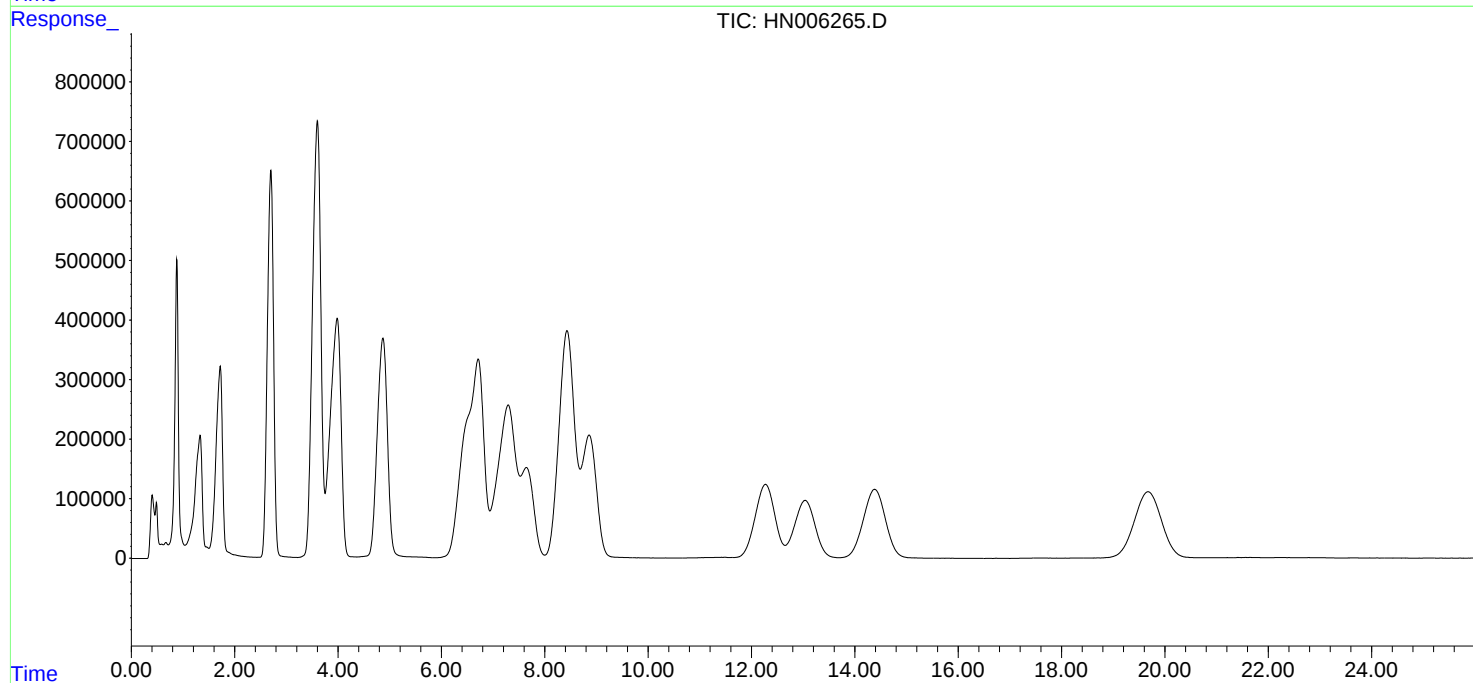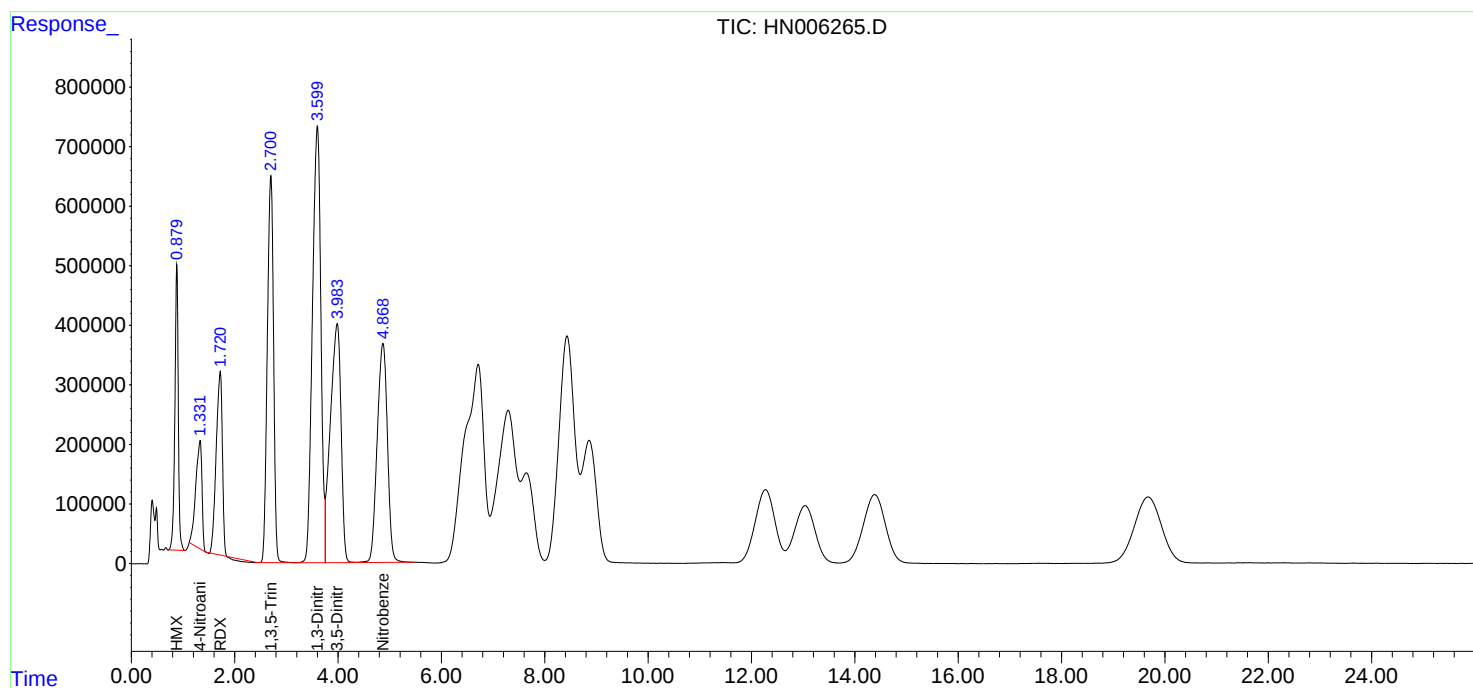


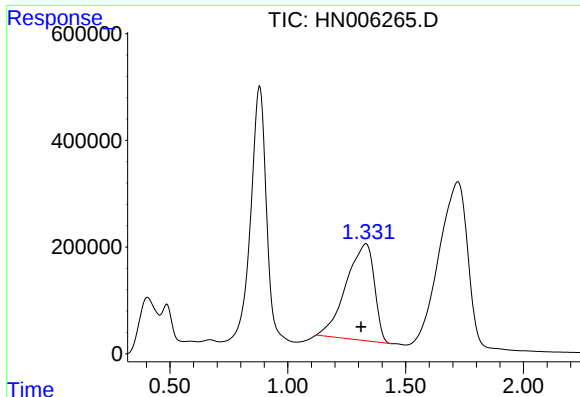

#1 4-Nitroaniline


R.T.: 1.331 min
Delta R.T.: 0.021 min
Response: 15013348
Conc: 4406.36 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDICC5000

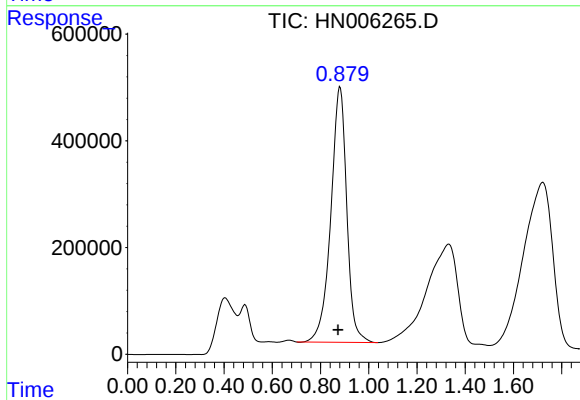


#2 HMX

R.T.: 0.881 min
Delta R.T.: 0.008 min
Response: 22002289
Conc: 4880.75 ug/L

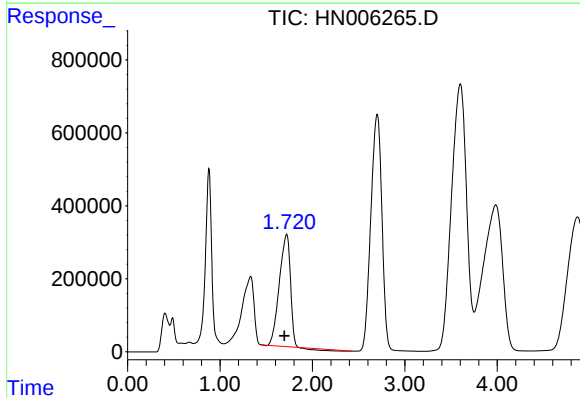


#3 RDX

R.T.: 1.722 min
Delta R.T.: 0.025 min
Response: 24822684
Conc: 4734.52 ug/L

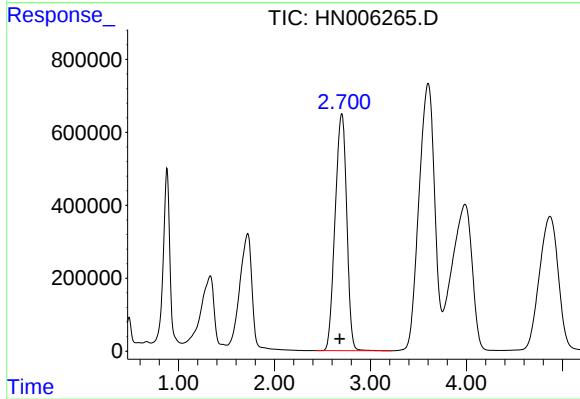

#4 1,3,5-Trinitrobenzene


R.T.: 2.701 min
Delta R.T.: 0.020 min
Response: 54578471
Conc: 5083.91 ug/L

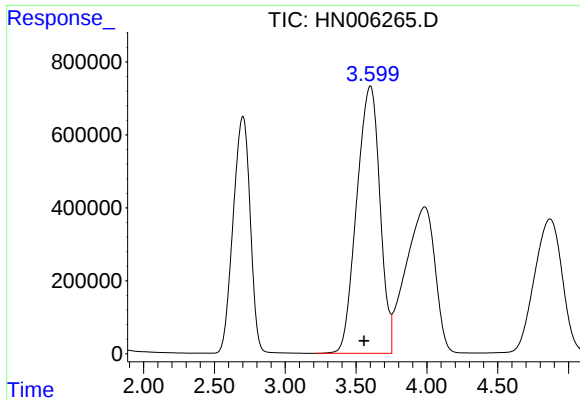

#5 1,3-Dinitrobenzene


R.T.: 3.601 min
Delta R.T.: 0.044 min
Response: 83542118
Conc: 5120.69 ng/ml

Instrument :
HPLC_N
ClientSampleId :
HSTDICC5000

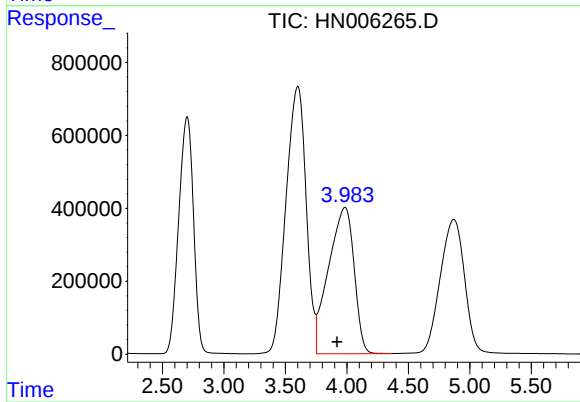

#6 3,5-Dinitroaniline

R.T.: 3.985 min
Delta R.T.: 0.065 min
Response: 57844579
Conc: 4975.10 ug/L

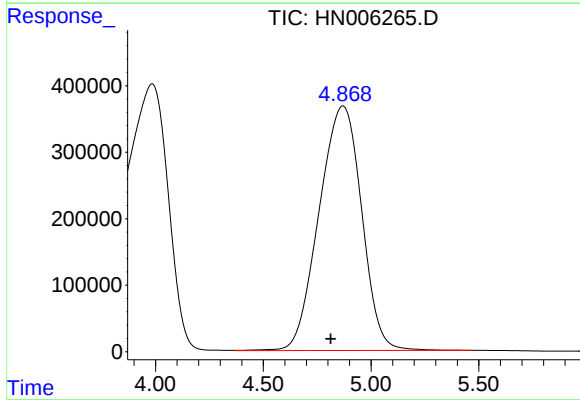

#7 Nitrobenzene

R.T.: 4.870 min
Delta R.T.: 0.056 min
Response: 50637077
Conc: 5028.15 ug/L