

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN100214\
 Data File : HN006266.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 02-Oct-2014, 10:44
 Operator : HNP
 Sample : HSTDICC2000
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 HSTDICC2000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 16:17:01 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
 Quant Title :
 QLast Update : Mon Mar 09 14:56:25 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.327	6491497	1905.231 ug/L
Target Compounds			
2) T HMX	0.880	8538575	1894.104 ug/L
3) T RDX	1.718	9900789	1888.411 ug/L
4) T 1,3,5-Trinitrobenzene	2.700	20831709	1940.445 ug/L
5) T 1,3-Dinitrobenzene	3.596	31365721	1922.553 ng/ml
6) T 3,5-Dinitroaniline	3.971f	22438827	1929.919 ug/L
7) T Nitrobenzene	4.865f	19346753	1921.092 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN100214\
Data File : HN006266.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 02-Oct-2014, 10:44
Operator : HNP
Sample : HSTDICC2000
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDICC2000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 16:17:01 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
Quant Title :
QLast Update : Mon Mar 09 14:56:25 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

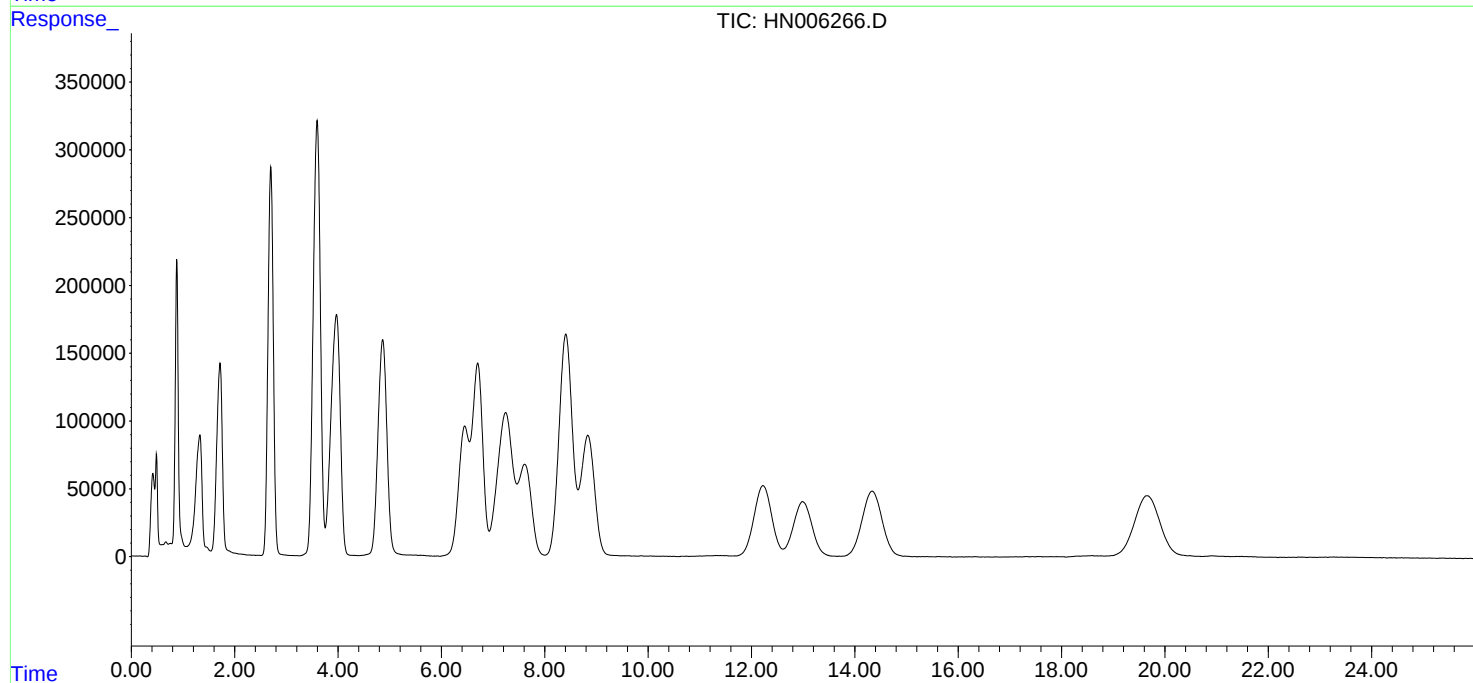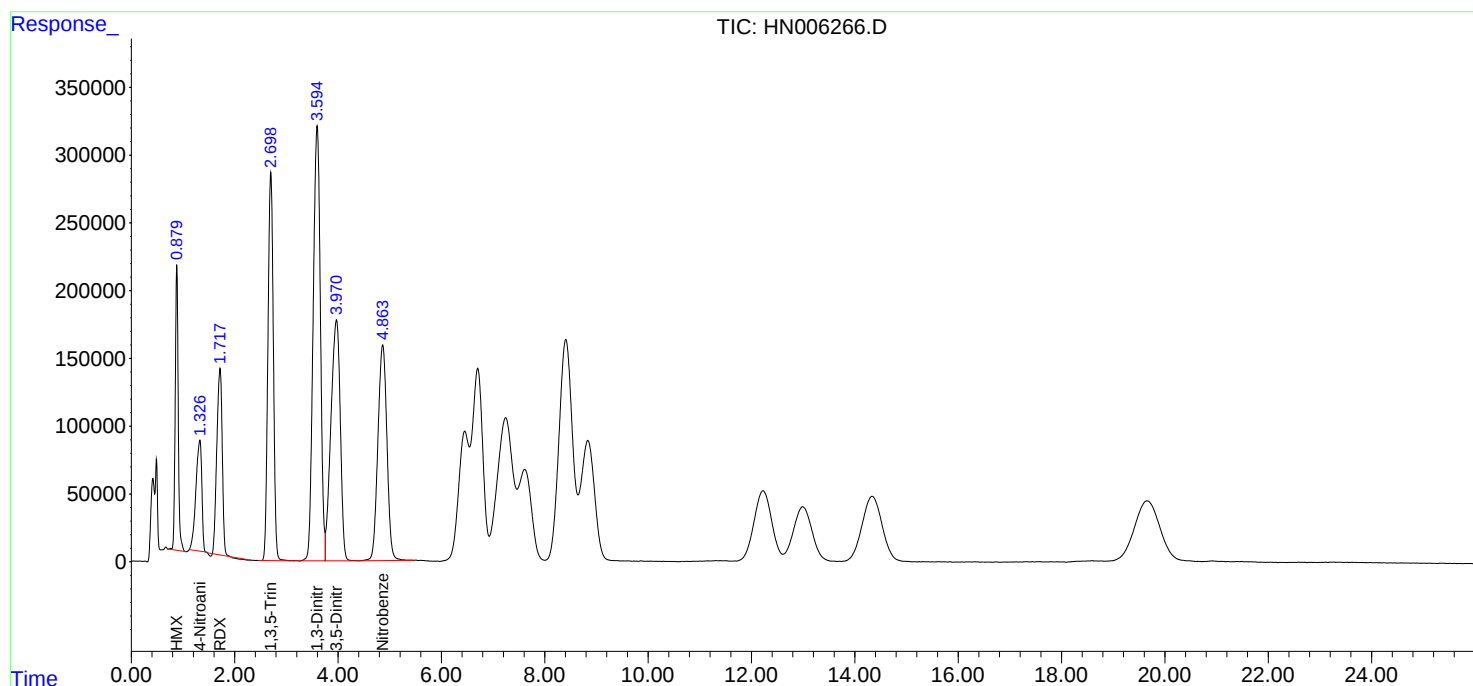


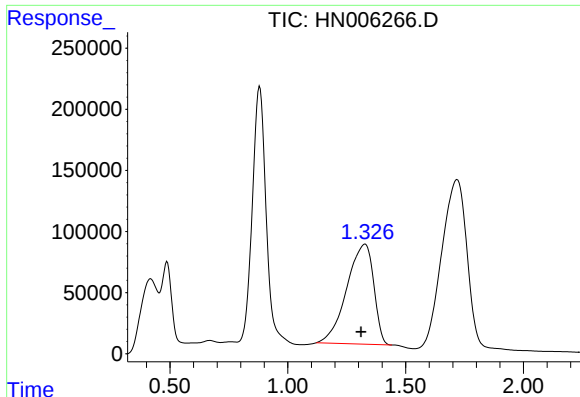

#1 4-Nitroaniline


R.T.: 1.327 min
Delta R.T.: 0.017 min
Response: 6491497
Conc: 1905.23 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDICC2000

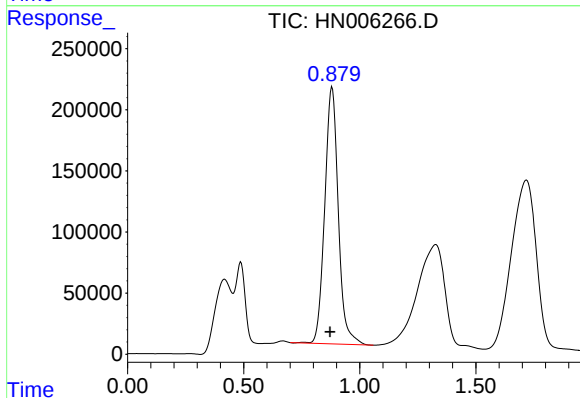


#2 HMX

R.T.: 0.880 min
Delta R.T.: 0.007 min
Response: 8538575
Conc: 1894.10 ug/L

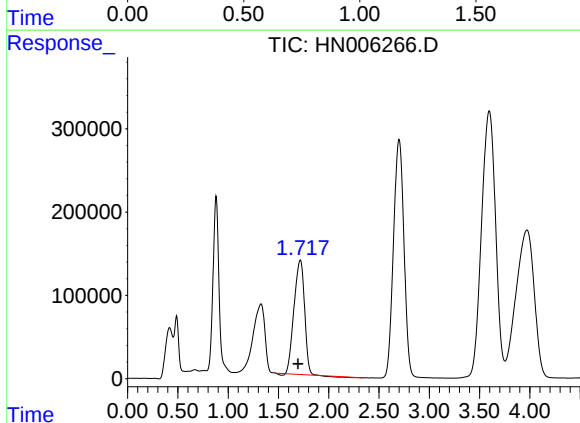


#3 RDX

R.T.: 1.718 min
Delta R.T.: 0.021 min
Response: 9900789
Conc: 1888.41 ug/L

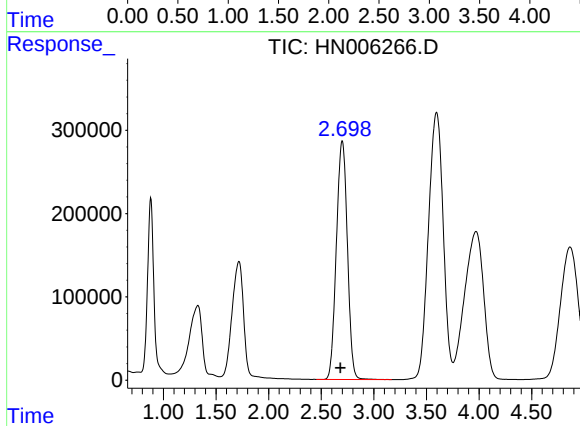

#4 1,3,5-Trinitrobenzene


R.T.: 2.700 min
Delta R.T.: 0.019 min
Response: 20831709
Conc: 1940.45 ug/L

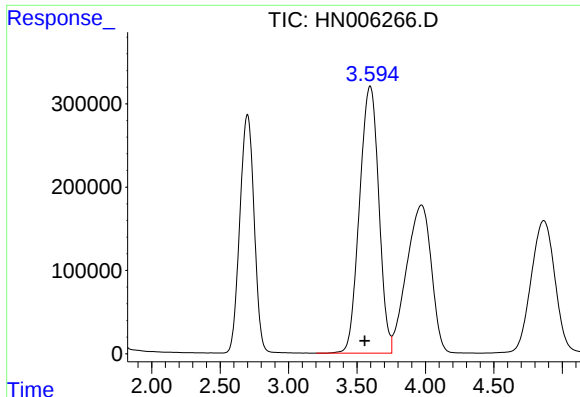

#5 1,3-Dinitrobenzene


R.T.: 3.596 min
Delta R.T.: 0.039 min
Response: 31365721
Conc: 1922.55 ng/ml

Instrument :
HPLC_N
ClientSampleId :
HSTDICC2000

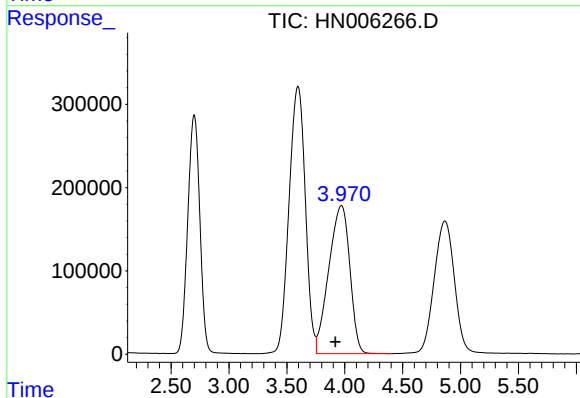

#6 3,5-Dinitroaniline

R.T.: 3.971 min
Delta R.T.: 0.051 min
Response: 22438827
Conc: 1929.92 ug/L

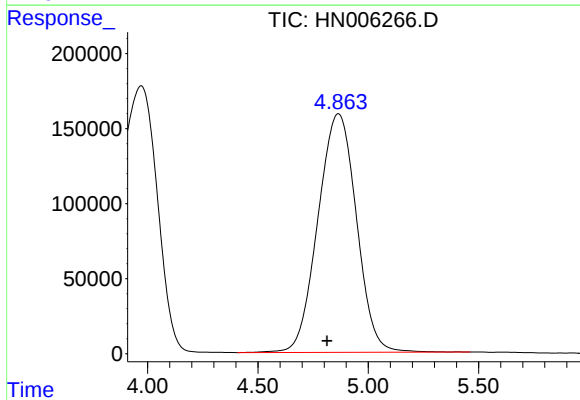

#7 Nitrobenzene

R.T.: 4.865 min
Delta R.T.: 0.051 min
Response: 19346753
Conc: 1921.09 ug/L