

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN100214\
 Data File : HN006267.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 02-Oct-2014, 11:12
 Operator : HNP
 Sample : HSTDICC1000
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 HSTDICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 16:17:27 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
 Quant Title :
 QLast Update : Mon Mar 09 14:56:25 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.330	3522775	1033.922 ug/L
Target Compounds			
2) T HMX	0.883	4616339	1024.038 ug/L
3) T RDX	1.722	5476980	1044.643 ug/L
4) T 1,3,5-Trinitrobenzene	2.703	11221425	1045.261 ug/L
5) T 1,3-Dinitrobenzene	3.599	16804469	1030.025 ng/ml
6) T 3,5-Dinitroaniline	3.972f	12006042	1032.616 ug/L
7) T Nitrobenzene	4.867f	10355421	1028.271 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN100214\
Data File : HN006267.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 02-Oct-2014, 11:12
Operator : HNP
Sample : HSTDICC1000
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 16:17:27 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
Quant Title :
QLast Update : Mon Mar 09 14:56:25 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

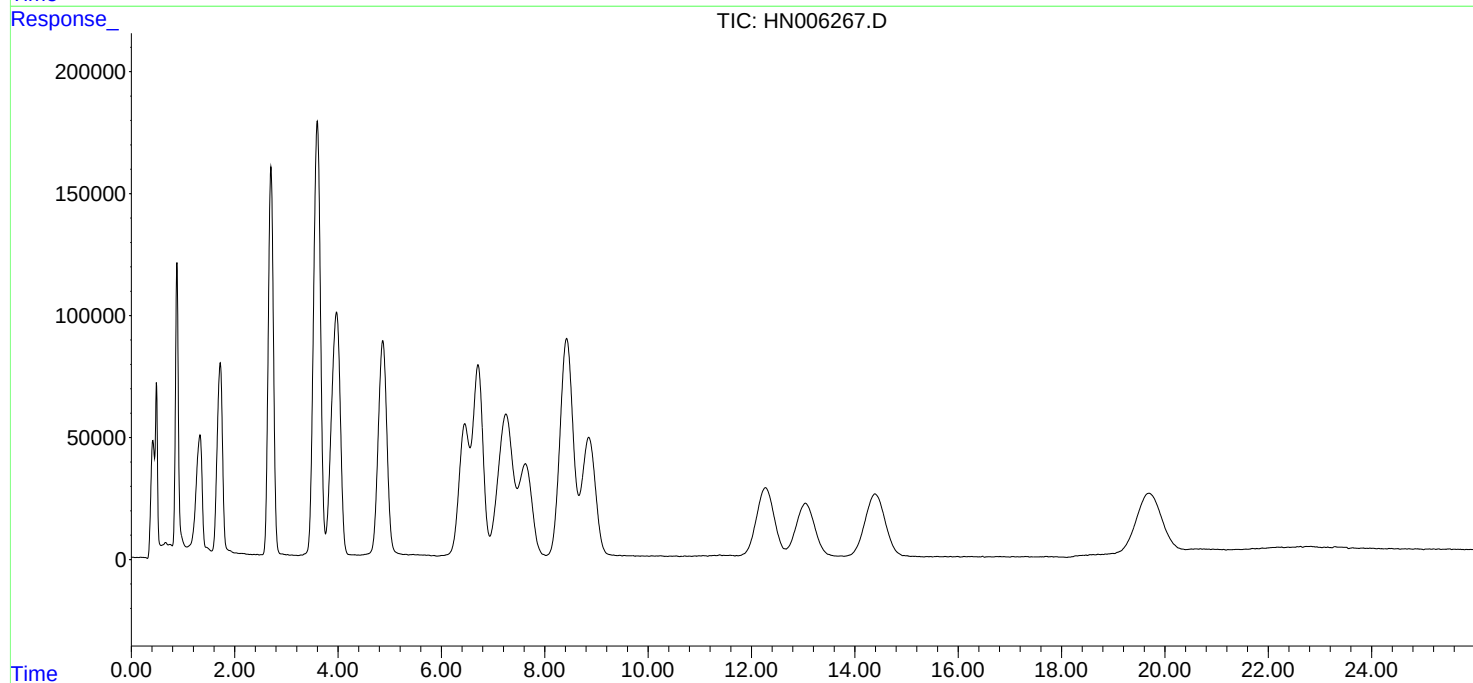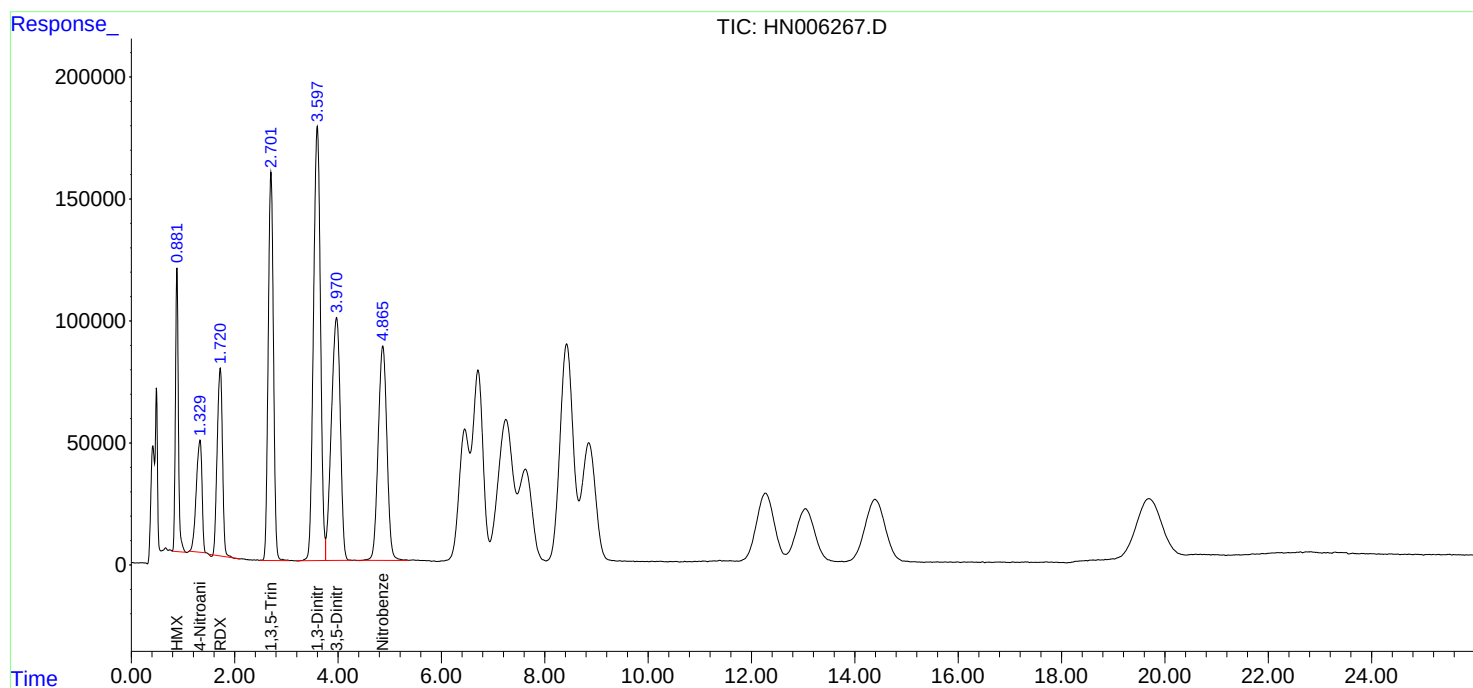


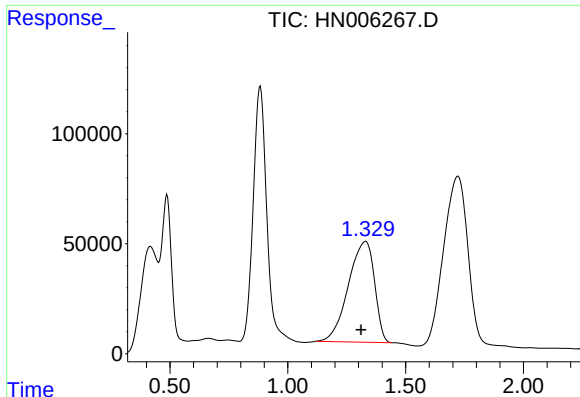

#1 4-Nitroaniline


R.T.: 1.330 min
Delta R.T.: 0.020 min
Response: 3522775
Conc: 1033.92 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDICC1000

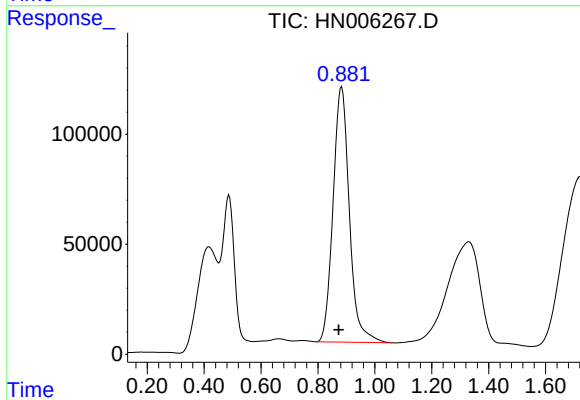


#2 HMX

R.T.: 0.883 min
Delta R.T.: 0.010 min
Response: 4616339
Conc: 1024.04 ug/L

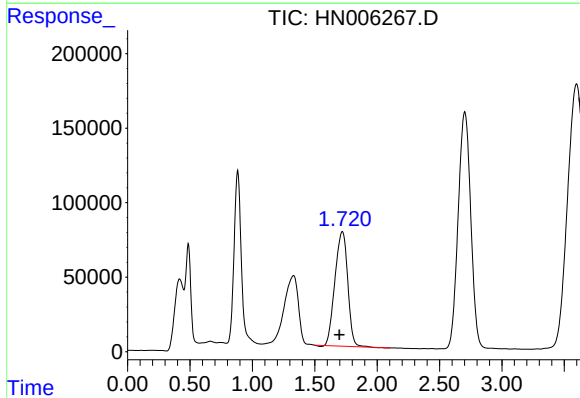


#3 RDX

R.T.: 1.722 min
Delta R.T.: 0.025 min
Response: 5476980
Conc: 1044.64 ug/L

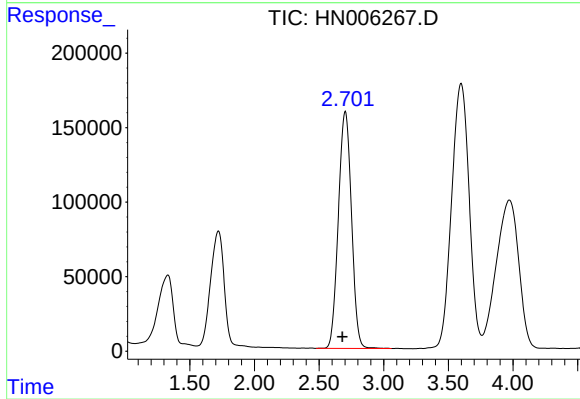

#4 1,3,5-Trinitrobenzene


R.T.: 2.703 min
Delta R.T.: 0.022 min
Response: 11221425
Conc: 1045.26 ug/L

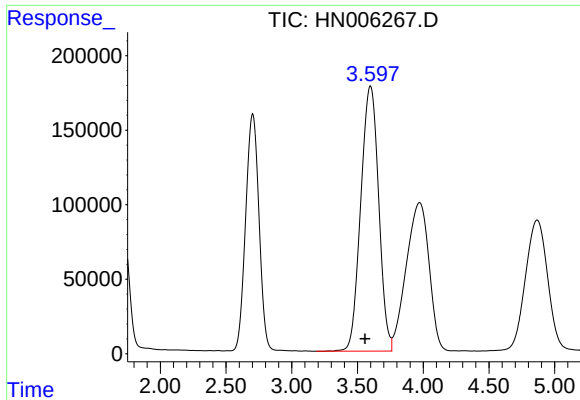

#5 1,3-Dinitrobenzene


R.T.: 3.599 min
Delta R.T.: 0.042 min
Response: 16804469
Conc: 1030.03 ng/ml

Instrument :
HPLC_N
ClientSampleId :
HSTDICC1000

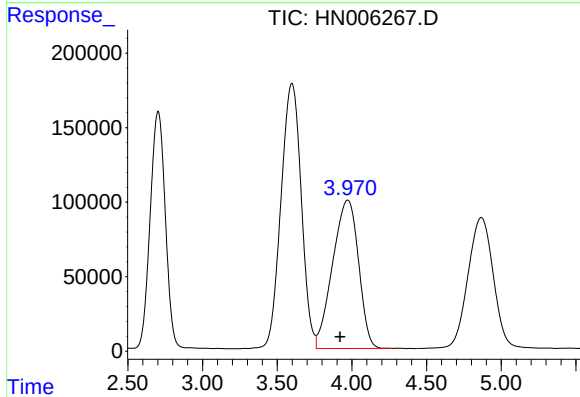

#6 3,5-Dinitroaniline

R.T.: 3.972 min
Delta R.T.: 0.052 min
Response: 12006042
Conc: 1032.62 ug/L

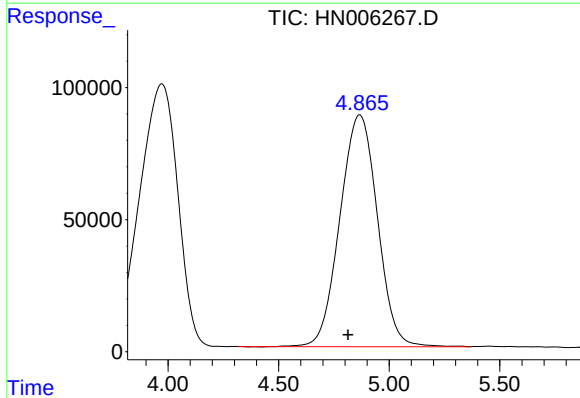

#7 Nitrobenzene

R.T.: 4.867 min
Delta R.T.: 0.053 min
Response: 10355421
Conc: 1028.27 ug/L