

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN100214\
 Data File : HN006268.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 02-Oct-2014, 11:41
 Operator : HNP
 Sample : HSTDICCC0500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 HSTDICCC0500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 16:17:37 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
 Quant Title :
 QLast Update : Mon Mar 09 14:56:25 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.327	1553533	455.956 ug/L
Target Compounds			
2) T HMX	0.882	1968270	436.619 ug/L
3) T RDX	1.722	2378363	453.633 ug/L
4) T 1,3,5-Trinitrobenzene	2.708	4807745	447.835 ug/L
5) T 1,3-Dinitrobenzene	3.608f	7298770	447.376 ng/ml
6) T 3,5-Dinitroaniline	3.984f	5221616	449.101 ug/L
7) T Nitrobenzene	4.884f	4575862	454.373 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN100214\
Data File : HN006268.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 02-Oct-2014, 11:41
Operator : HNP
Sample : HSTDICCC0500
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDICCC0500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 16:17:37 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
Quant Title :
QLast Update : Mon Mar 09 14:56:25 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

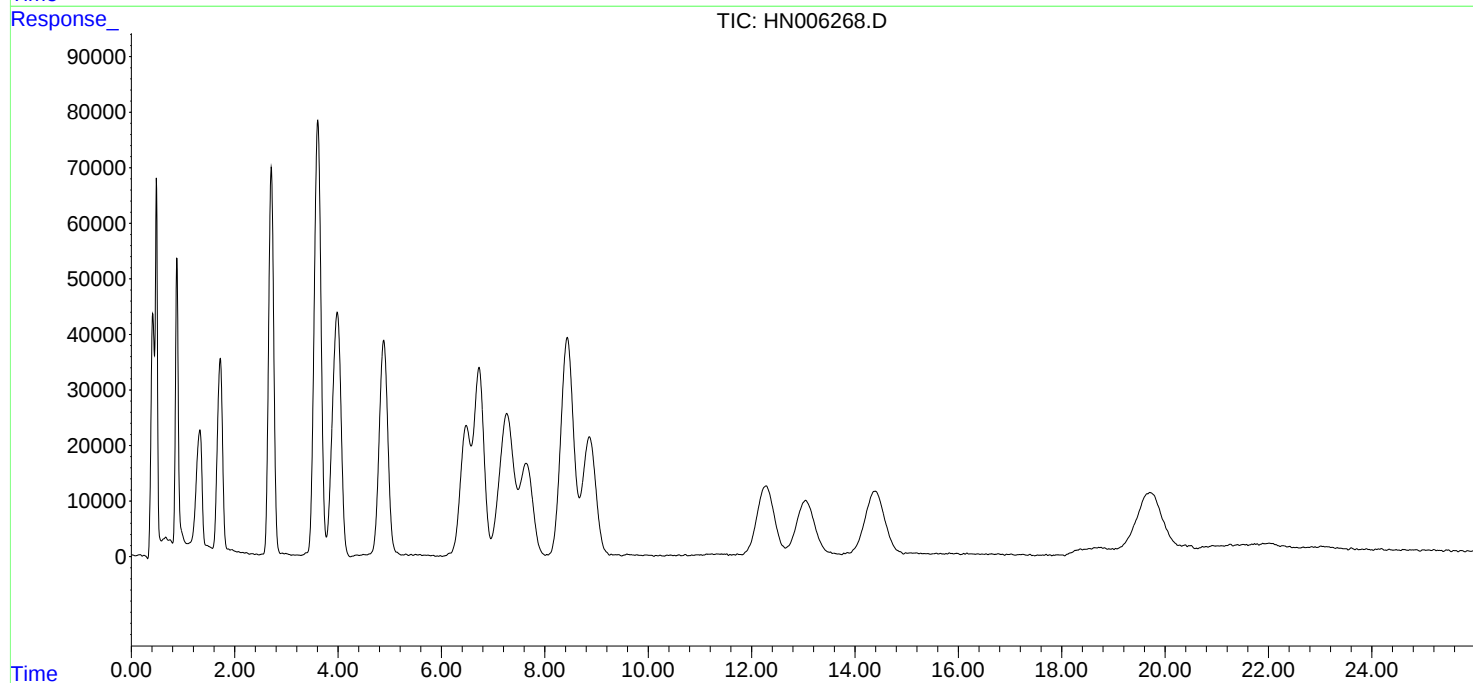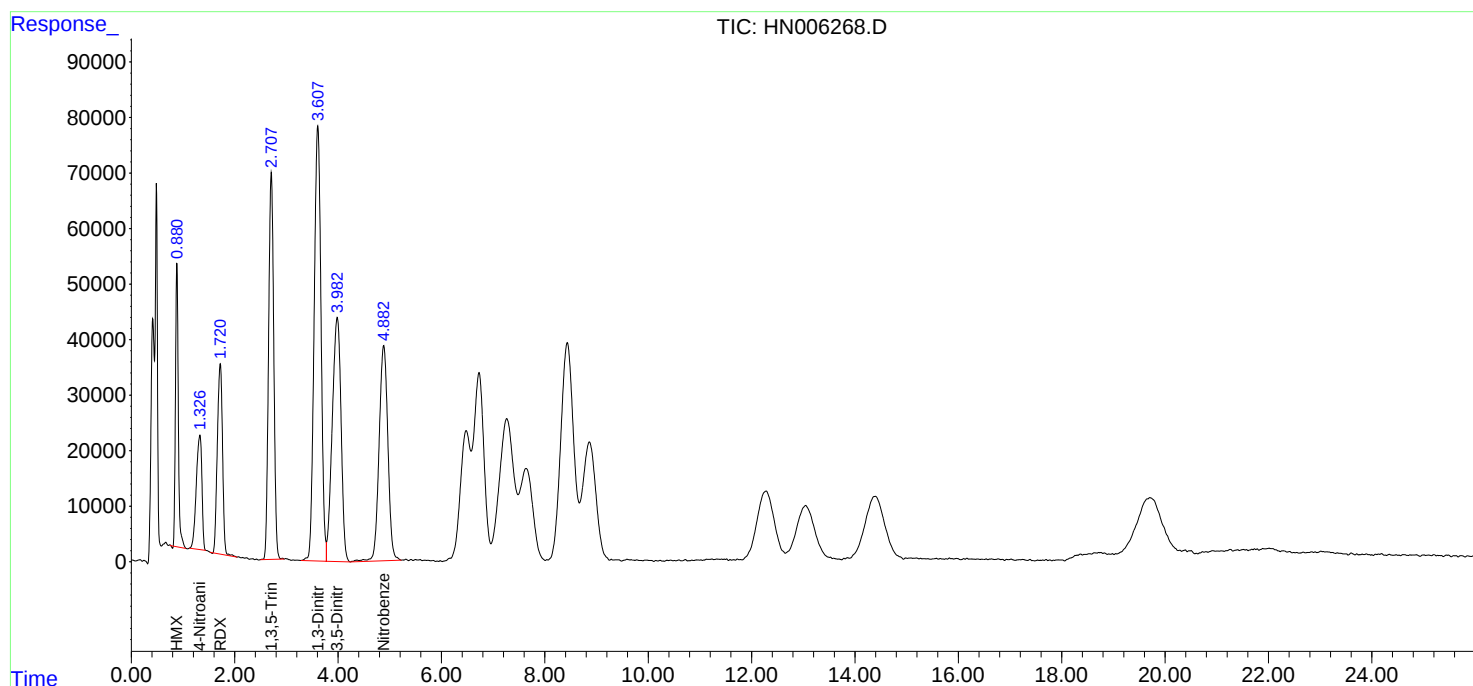


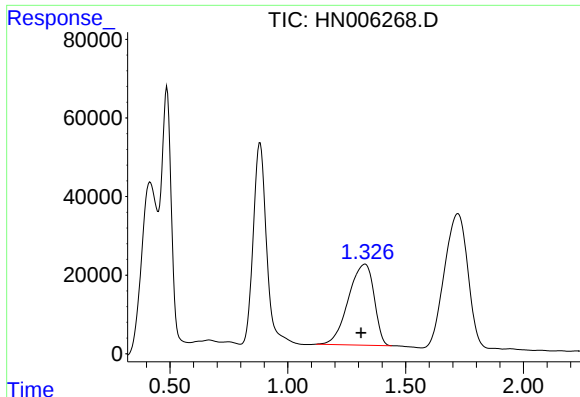

#1 4-Nitroaniline


R.T.: 1.327 min
Delta R.T.: 0.017 min
Response: 1553533
Conc: 455.96 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDICCC0500

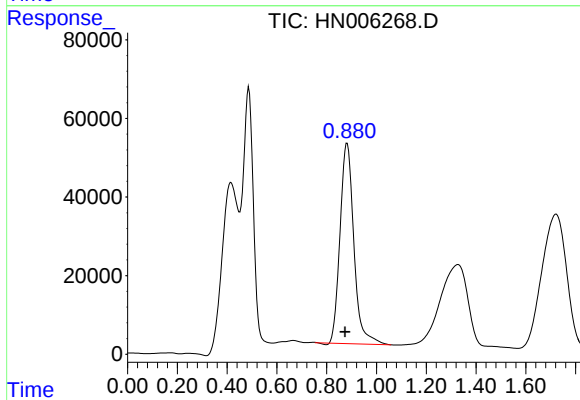


#2 HMX

R.T.: 0.882 min
Delta R.T.: 0.009 min
Response: 1968270
Conc: 436.62 ug/L

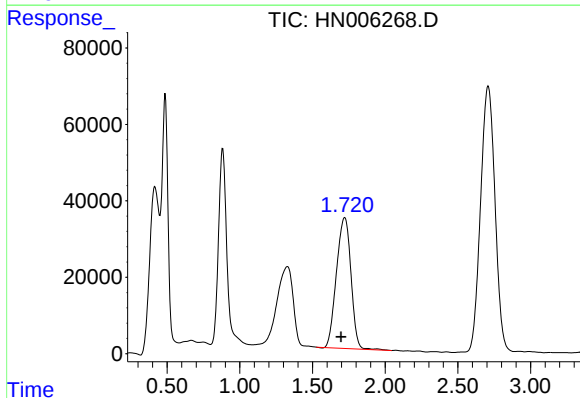


#3 RDX

R.T.: 1.722 min
Delta R.T.: 0.025 min
Response: 2378363
Conc: 453.63 ug/L

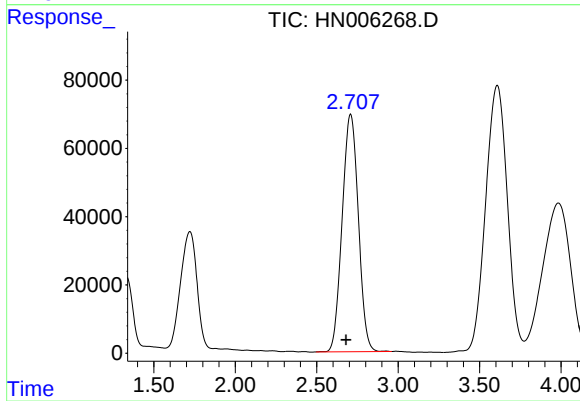

#4 1,3,5-Trinitrobenzene


R.T.: 2.708 min
Delta R.T.: 0.028 min
Response: 4807745
Conc: 447.83 ug/L

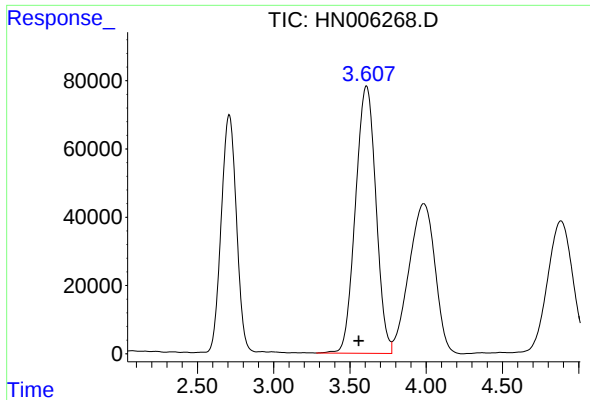

#5 1,3-Dinitrobenzene


R.T.: 3.608 min
Delta R.T.: 0.051 min
Response: 7298770
Conc: 447.38 ng/ml

Instrument :
HPLC_N
ClientSampleId :
HSTDICCC0500

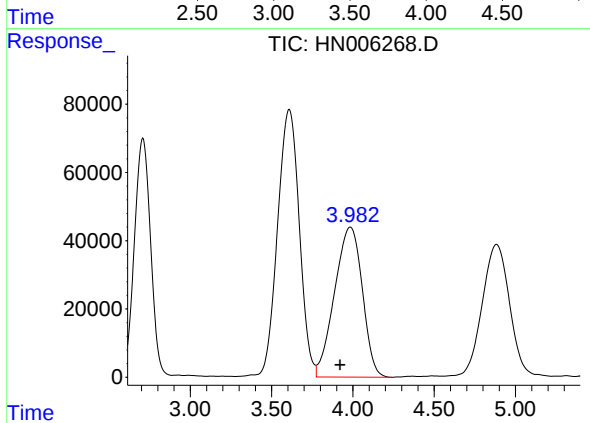

#6 3,5-Dinitroaniline

R.T.: 3.984 min
Delta R.T.: 0.064 min
Response: 5221616
Conc: 449.10 ug/L

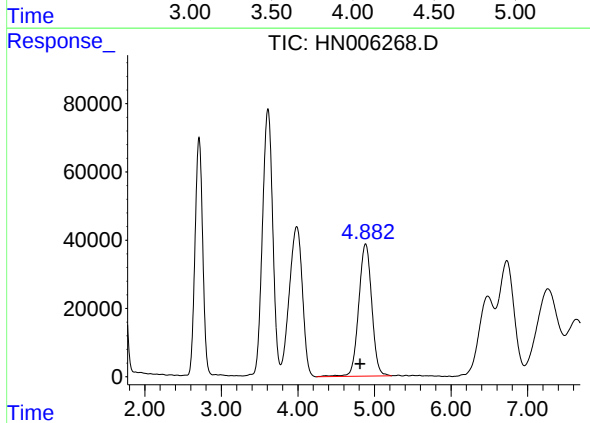

#7 Nitrobenzene

R.T.: 4.884 min
Delta R.T.: 0.070 min
Response: 4575862
Conc: 454.37 ug/L