

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN100214\
 Data File : HN006272.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 02-Oct-2014, 13:33
 Operator : HNP
 Sample : PB79088BS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 PB79088BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 16:18:15 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
 Quant Title :
 QLast Update : Mon Mar 09 14:56:25 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.325	1387666	407.275 ug/L
Target Compounds			
2) T HMX	0.884	1162069	257.781 ug/L
3) T RDX	1.722	1443963	275.412 ug/L
4) T 1,3,5-Trinitrobenzene	2.715	2729226	254.224 ug/L
5) T 1,3-Dinitrobenzene	3.617f	4323766	265.024 ng/ml
6) T 3,5-Dinitroaniline	3.990f	3188760	274.259 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN100214\
Data File : HN006272.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 02-Oct-2014, 13:33
Operator : HNP
Sample : PB79088BS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
PB79088BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 16:18:15 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
Quant Title :
QLast Update : Mon Mar 09 14:56:25 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

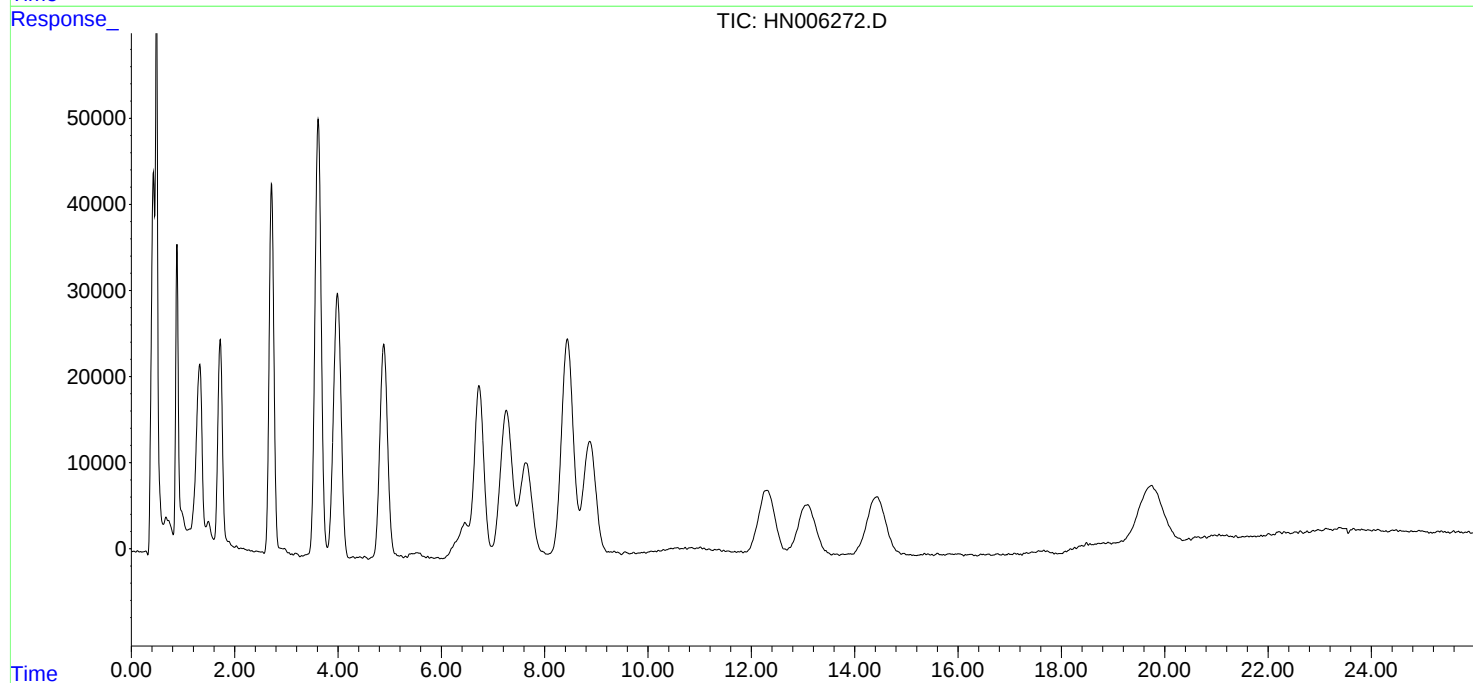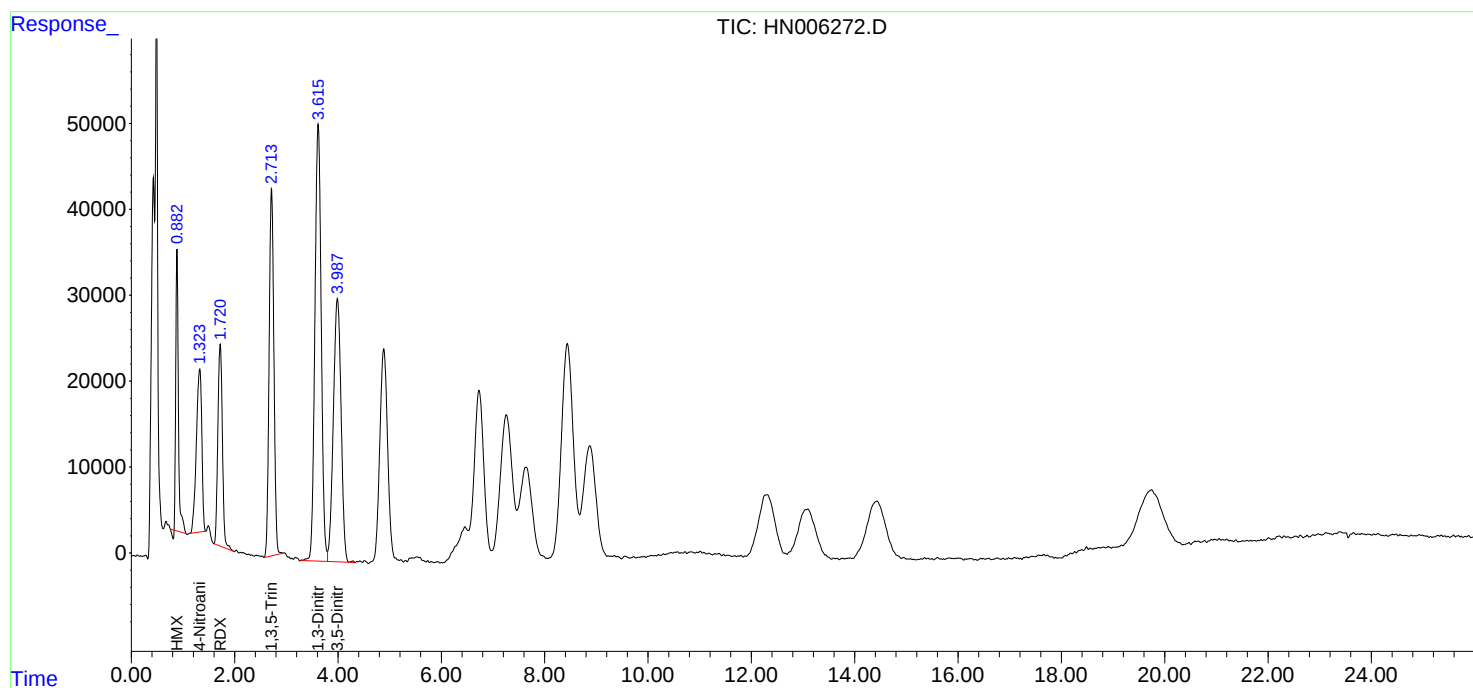


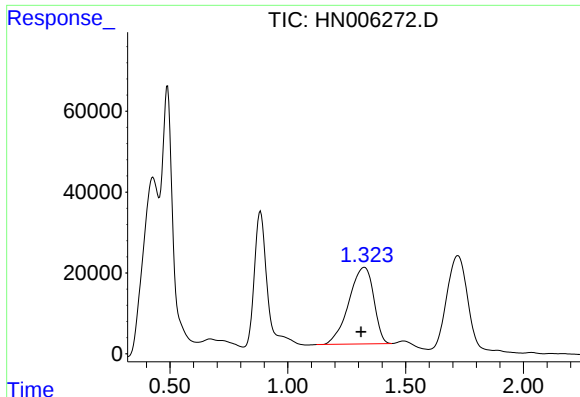

#1 4-Nitroaniline


R.T.: 1.325 min
Delta R.T.: 0.015 min
Response: 1387666
Conc: 407.27 ug/L

Instrument :
HPLC_N
ClientSampleId :
PB79088BS

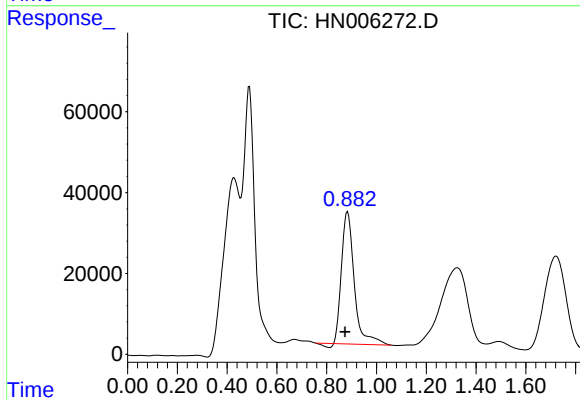


#2 HMX

R.T.: 0.884 min
Delta R.T.: 0.011 min
Response: 1162069
Conc: 257.78 ug/L

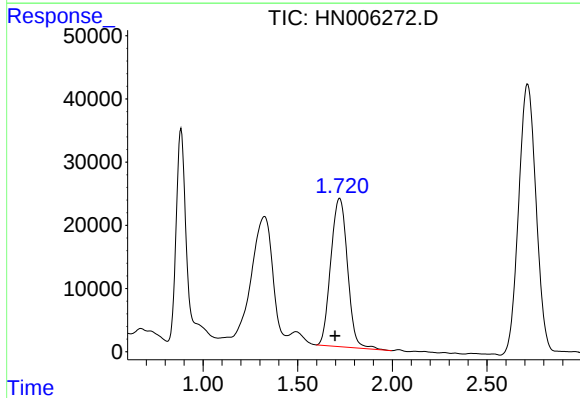


#3 RDX

R.T.: 1.722 min
Delta R.T.: 0.025 min
Response: 1443963
Conc: 275.41 ug/L

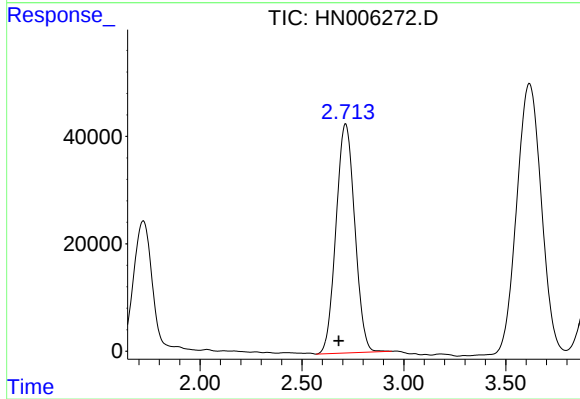

#4 1,3,5-Trinitrobenzene


R.T.: 2.715 min
Delta R.T.: 0.034 min
Response: 2729226
Conc: 254.22 ug/L

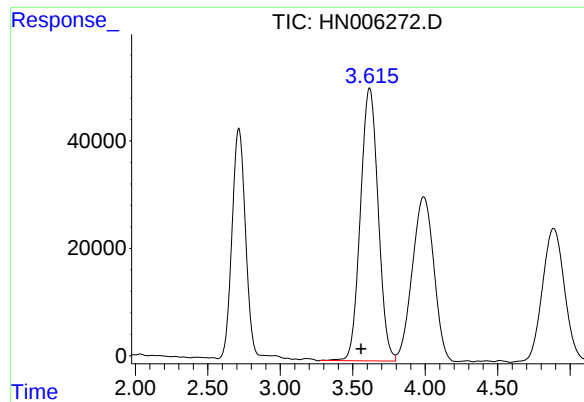

#5 1,3-Dinitrobenzene

R.T.: 3.617 min
Delta R.T.: 0.059 min
Response: 4323766
Conc: 265.02 ng/ml

Instrument :
HPLC_N
ClientSampleId :
PB79088BS

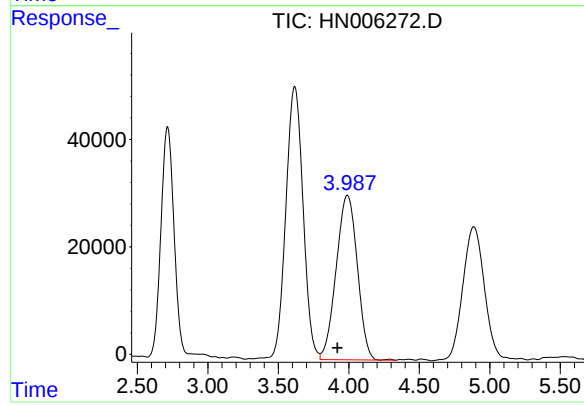

#6 3,5-Dinitroaniline

R.T.: 3.990 min
Delta R.T.: 0.069 min
Response: 3188760
Conc: 274.26 ug/L