

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN100214\
 Data File : HN006274.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 02-Oct-2014, 14:29
 Operator : HNP
 Sample : HSTDCCC0500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 HSTDCCC0500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 16:18:32 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
 Quant Title :
 QLast Update : Mon Mar 09 14:56:25 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.328	1617396	474.700 ug/L
Target Compounds			
2) T HMX	0.883	2041898	452.952 ug/L
3) T RDX	1.722	2400990	457.949 ug/L
4) T 1,3,5-Trinitrobenzene	2.709	4891183	455.607 ug/L
5) T 1,3-Dinitrobenzene	3.608f	7399751	453.566 ng/ml
6) T 3,5-Dinitroaniline	3.982f	5264770	452.812 ug/L
7) T Nitrobenzene	4.883f	4667569	463.480 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN100214\
Data File : HN006274.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 02-Oct-2014, 14:29
Operator : HNP
Sample : HSTDCCC0500
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 16:18:32 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
Quant Title :
QLast Update : Mon Mar 09 14:56:25 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

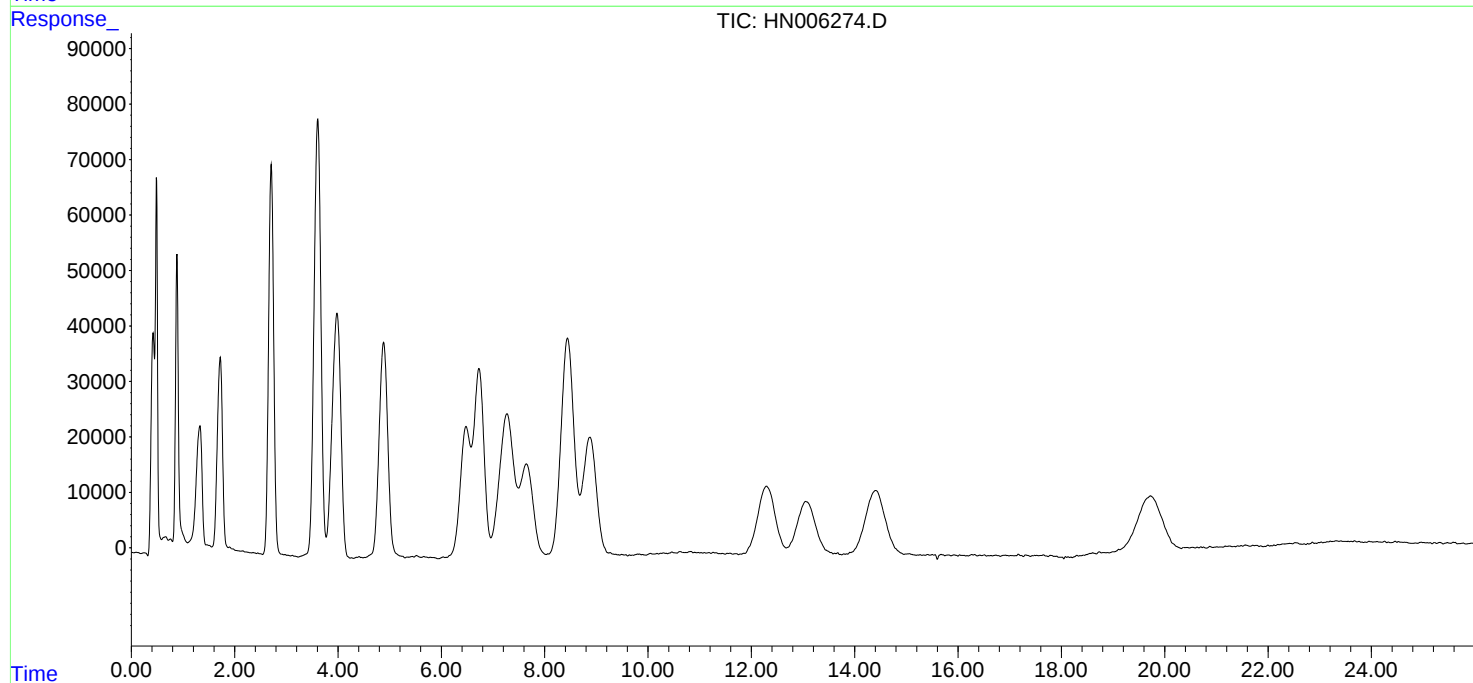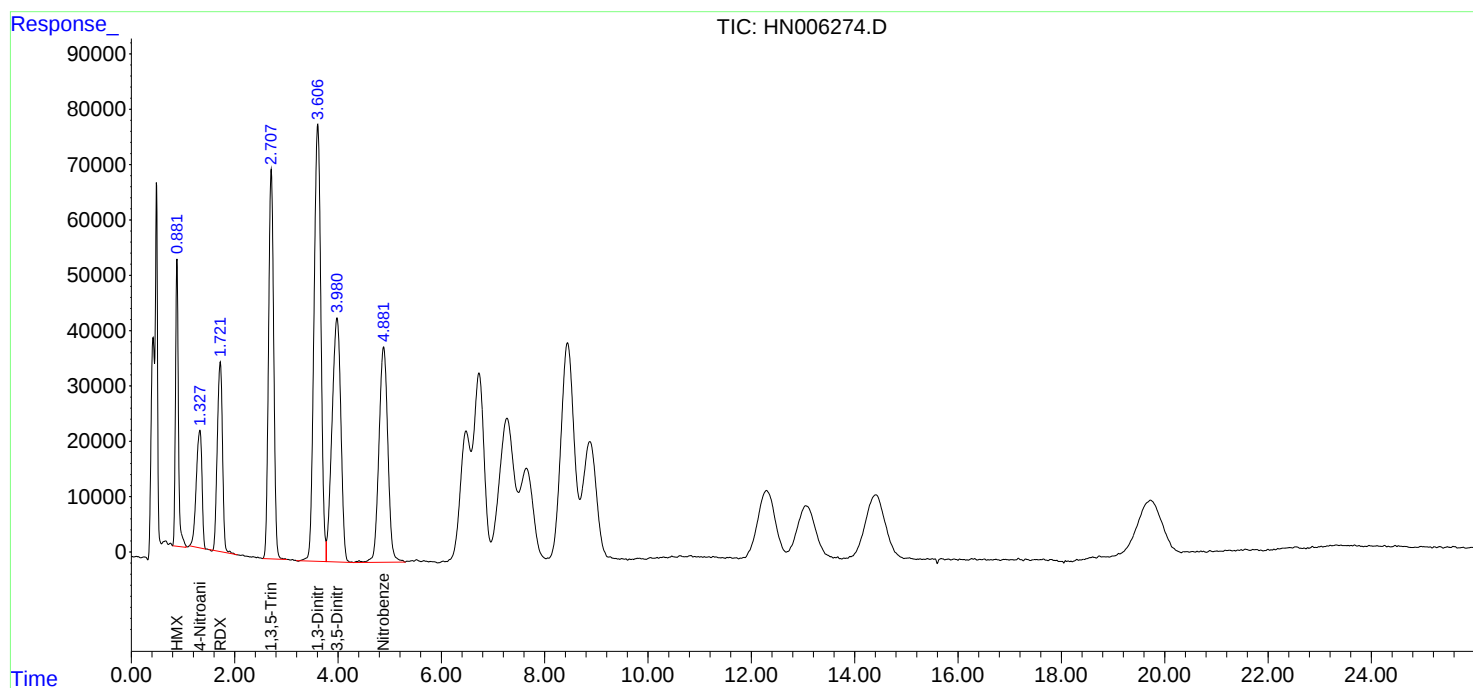


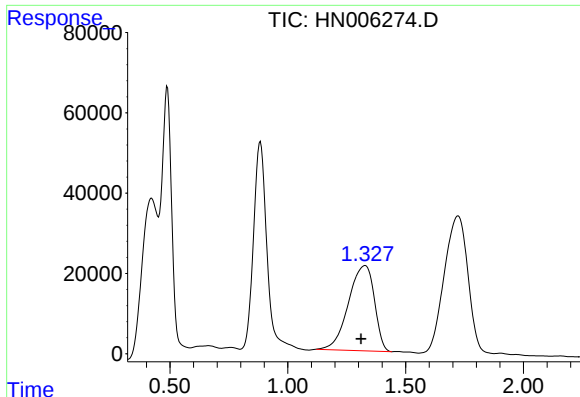

#1 4-Nitroaniline


R.T.: 1.328 min
Delta R.T.: 0.018 min
Response: 1617396
Conc: 474.70 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

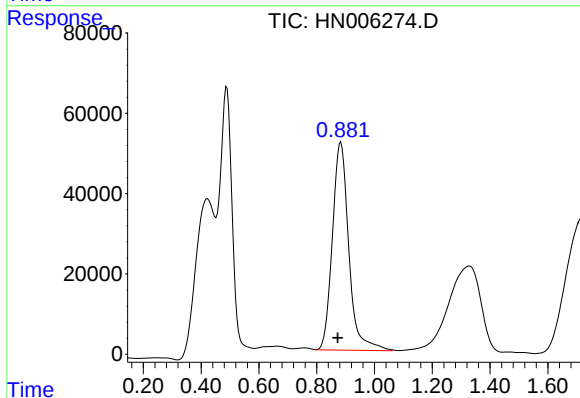


#2 HMX

R.T.: 0.883 min
Delta R.T.: 0.010 min
Response: 2041898
Conc: 452.95 ug/L

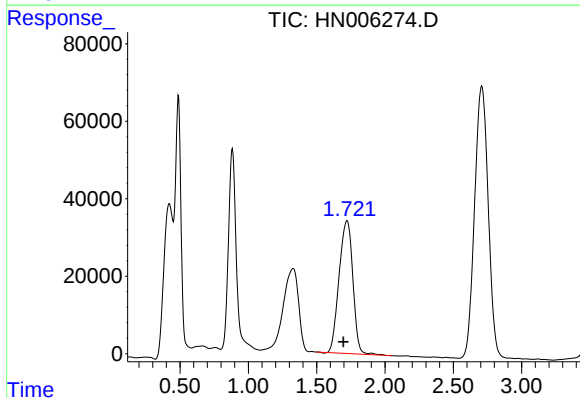


#3 RDX

R.T.: 1.722 min
Delta R.T.: 0.025 min
Response: 2400990
Conc: 457.95 ug/L

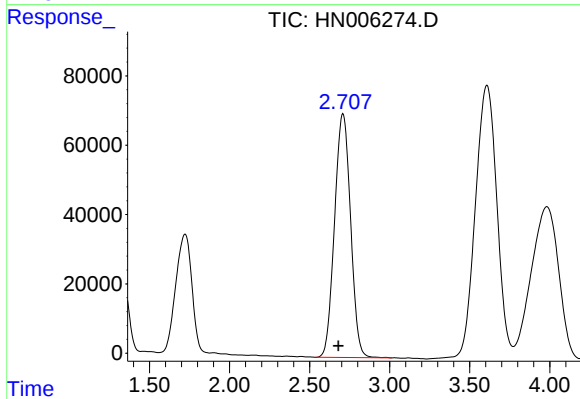

#4 1,3,5-Trinitrobenzene


R.T.: 2.709 min
Delta R.T.: 0.028 min
Response: 4891183
Conc: 455.61 ug/L

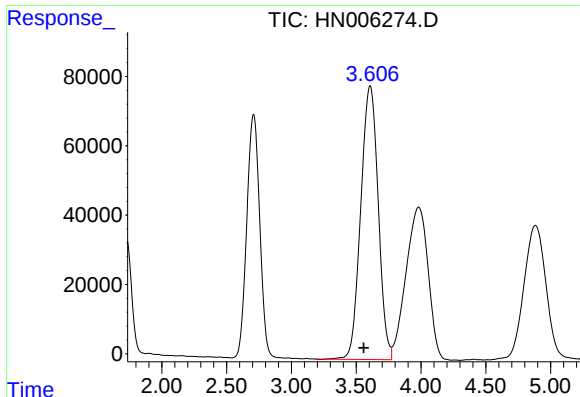

#5 1,3-Dinitrobenzene


R.T.: 3.608 min
Delta R.T.: 0.051 min
Response: 7399751
Conc: 453.57 ng/ml

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

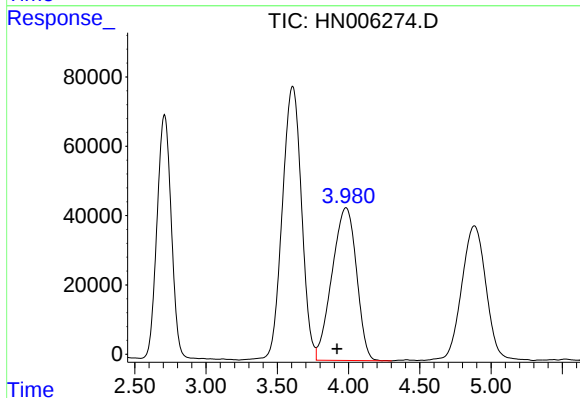

#6 3,5-Dinitroaniline

R.T.: 3.982 min
Delta R.T.: 0.062 min
Response: 5264770
Conc: 452.81 ug/L

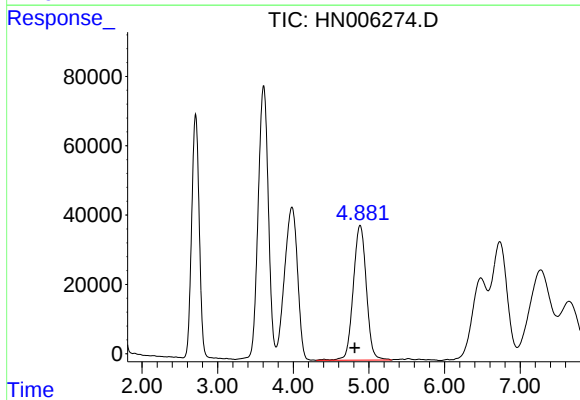

#7 Nitrobenzene

R.T.: 4.883 min
Delta R.T.: 0.069 min
Response: 4667569
Conc: 463.48 ug/L