

Data Path : Z:\HPCHEM1\HPLC\_N\Data\HN100316\  
Data File : HN007773.D  
Signal(s) : vwd1A.ch  
Acq On : 03-Oct-2016, 11:27  
Operator : UM/MA  
Sample : HSTDCCC005  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
HPLC\_N  
ClientSampleId :  
HSTDCCC005

Manual Integrations  
APPROVED

umangi  
10/4/2016 7:10:48 PM

Integration File: AUTOINT1.E  
Quant Time: Oct 06 16:22:14 2016  
Quant Method : Z:\HPCHEM1\HPLC\_N\Methods\HN092716NG.M  
Quant Title :  
QLast Update : Thu Oct 06 16:22:06 2016  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

| Compound                    | R.T.  | Response | Conc Units  |
|-----------------------------|-------|----------|-------------|
| -----                       |       |          |             |
| System Monitoring Compounds |       |          |             |
| 1) S 4-Nitroaniline         | 1.346 | 20199477 | 5.131 ng/ul |
| Target Compounds            |       |          |             |
| 2) T Nitroglycerin          | 6.052 | 42887810 | 5.160 ng/ul |
| -----                       |       |          |             |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\HPCHEM1\HPLC\_N\Data\HN100316\  
Data File : HN007773.D  
Signal(s) : vwd1A.ch  
Acq On : 03-Oct-2016, 11:27  
Operator : UM/MA  
Sample : HSTDCCC005  
Misc :  
ALS Vial : 1 Sample Multiplier: 1


Instrument :  
HPLC\_N  
ClientSampleId :  
HSTDCCC005


Manual Integrations  
APPROVED

umangi  
10/4/2016 7:10:48 PM

Integration File: AUTOINT1.E  
Quant Time: Oct 06 16:22:14 2016  
Quant Method : Z:\HPCHEM1\HPLC\_N\Methods\HN092716NG.M  
Quant Title :  
QLast Update : Thu Oct 06 16:22:06 2016  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

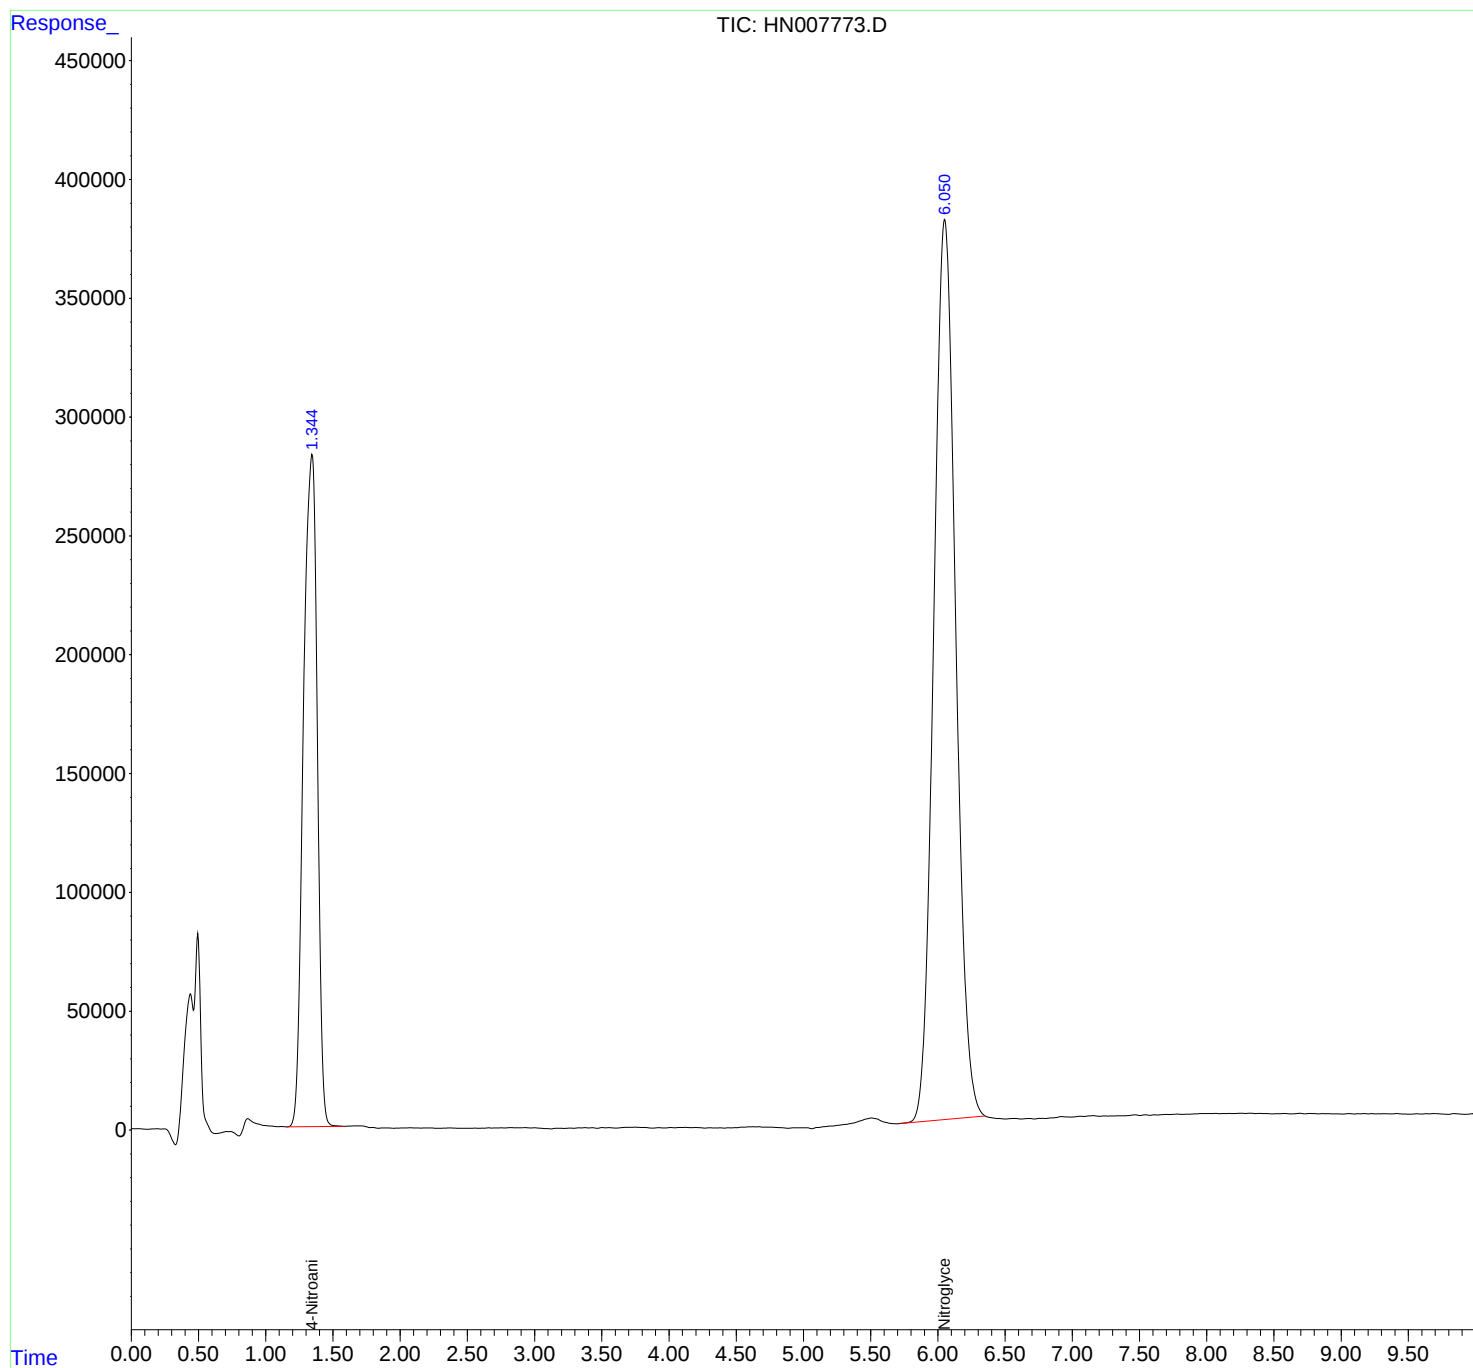

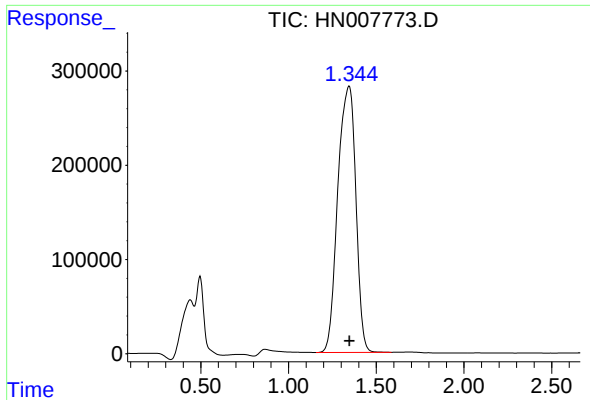


#1 4-Nitroaniline

R.T.: 1.346 min  
Delta R.T.: 0.000 min  
Response: 20199477  
Conc: 5.13 ng/ul

Instrument :  
HPLC\_N  
ClientSampleId :  
HSTDCCC005

Manual Integrations  
APPROVED

umangi  
10/4/2016 7:10:48 PM

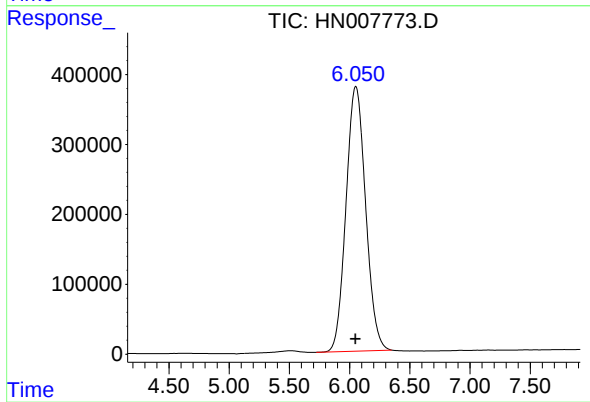

#2 Nitroglycerin

R.T.: 6.052 min  
Delta R.T.: 0.002 min  
Response: 42887810  
Conc: 5.16 ng/ul