

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN100515\
 Data File : HN007552.D
 Signal(s) : vwd1A.ch
 Acq On : 05-Oct-2015, 13:06
 Operator : UM/MA
 Sample : SSTDICCC0500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 SSTDICCC0500

Integration File: autoint1.e
 Quant Time: Oct 05 14:15:08 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN100515.M
 Quant Title :
 QLast Update : Mon Oct 05 14:14:48 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.326	1895131	500.000 ug/L
Target Compounds			
2) T HMX	0.892	2414393	500.000 ug/L
3) T RDX	1.710	2830062	500.000 ug/L
4) T 1,3,5-Trinitrobenzene	2.643	5883206	500.000 ug/L
5) T 1,3-Dinitrobenzene	3.517	8493404	500.000 ng/ml
6) T 3,5-Dinitroaniline	3.914	6159773	500.000 ug/L
7) T Nitrobenzene	4.692	5038872	500.000 ug/L
8) T Tetryl	6.249	3774085	500.000 ug/L
9) T 2,4,6-Trinitrotoluene	6.457	5958008	500.000 ug/L
10) T 2-Amino-4,6-dinitroto...	7.058	5480711	500.000 ug/L
11) T 4-Amino-2,6-dinitroto...	7.407	3527012	500.000 ug/L
12) T 2,4-Dinitrotoluene	8.089	7650239	500.000 ug/L
13) T 2,6-Dinitrotoluene	8.485	4348716	500.000 ug/L
14) T 2-Nitrotoluene	11.600	3219116	500.000 ug/L
15) T 4-Nitrotoluene	12.342	2666014	500.000 ug/L
16) T 3-Nitrotoluene	13.597	3402565	500.000 ug/L
17) T PETN	18.777	3896023	500.000 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN100515\
Data File : HN007552.D
Signal(s) : vwd1A.ch
Acq On : 05-Oct-2015, 13:06
Operator : UM/MA
Sample : SSTDICCC0500
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
SSTDICCC0500

Integration File: autoint1.e
Quant Time: Oct 05 14:15:08 2015
Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN100515.M
Quant Title :
QLast Update : Mon Oct 05 14:14:48 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

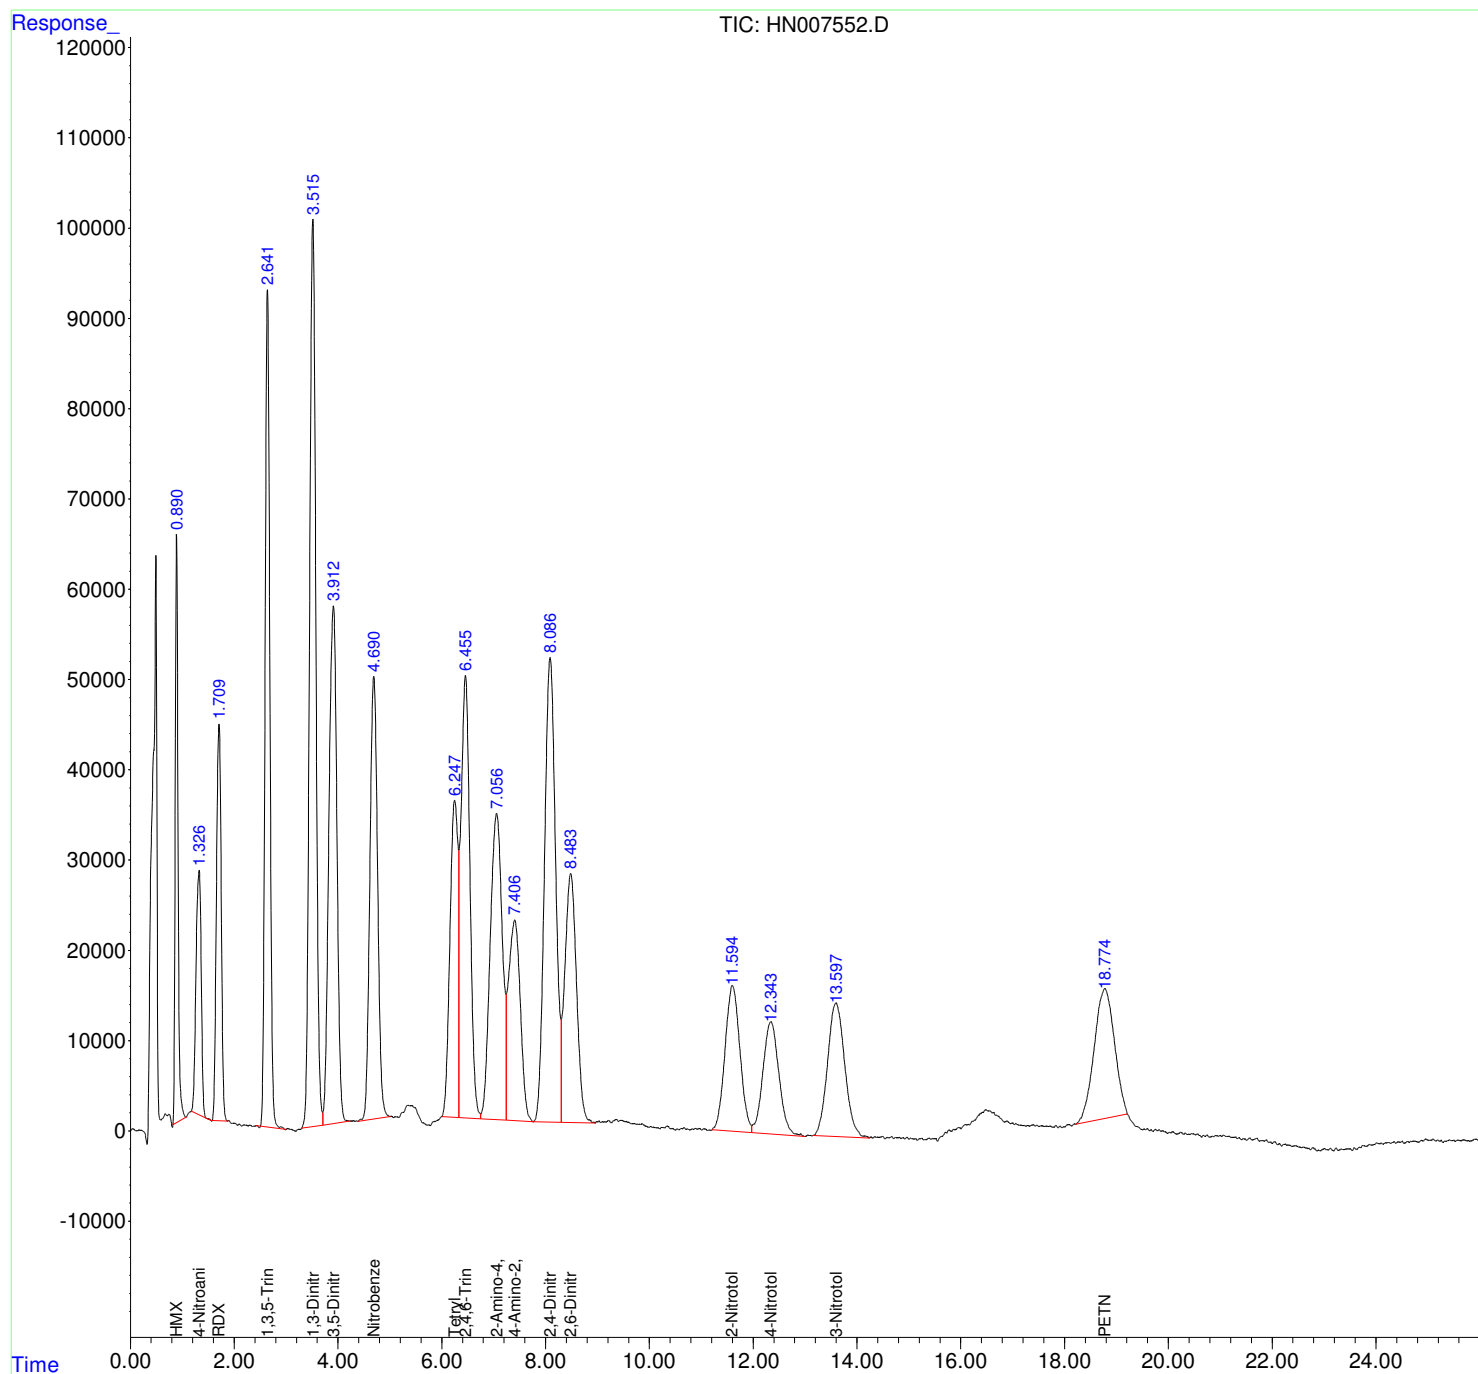


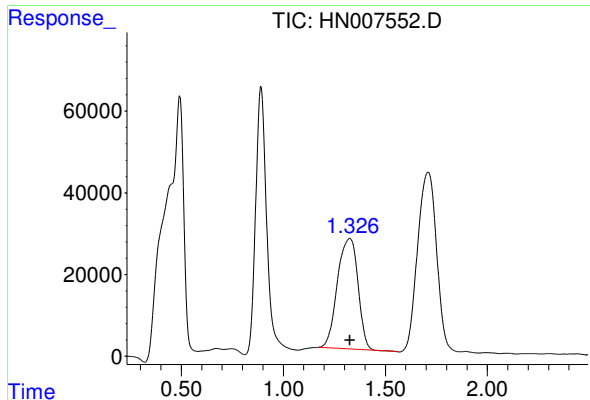

#1 4-Nitroaniline


R.T.: 1.326 min
Delta R.T.: 0.000 min
Response: 1895131
Conc: 500.00 ug/L

Instrument :
HPLC_N
ClientSampleId :
SSTDICCC0500

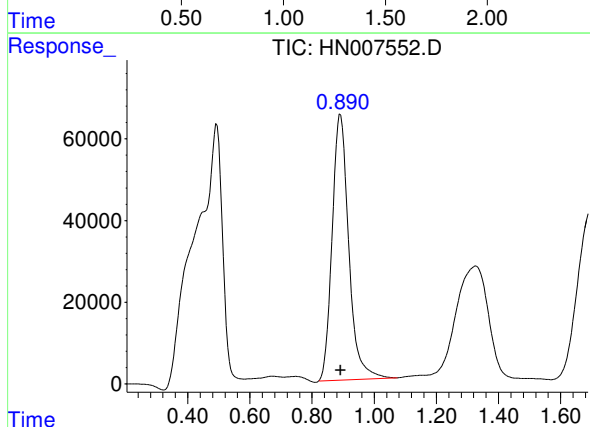


#2 HMX

R.T.: 0.892 min
Delta R.T.: 0.000 min
Response: 2414393
Conc: 500.00 ug/L

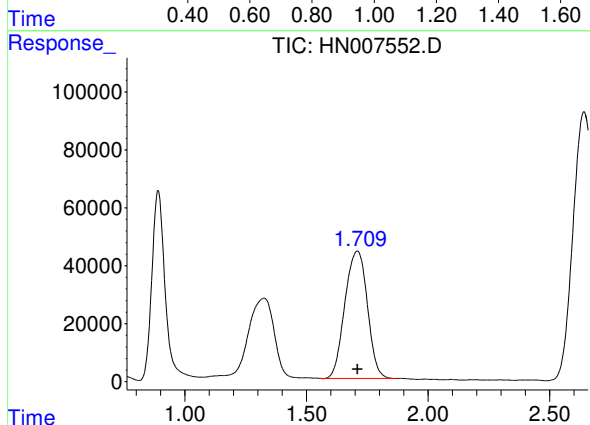


#3 RDX

R.T.: 1.710 min
Delta R.T.: 0.000 min
Response: 2830062
Conc: 500.00 ug/L

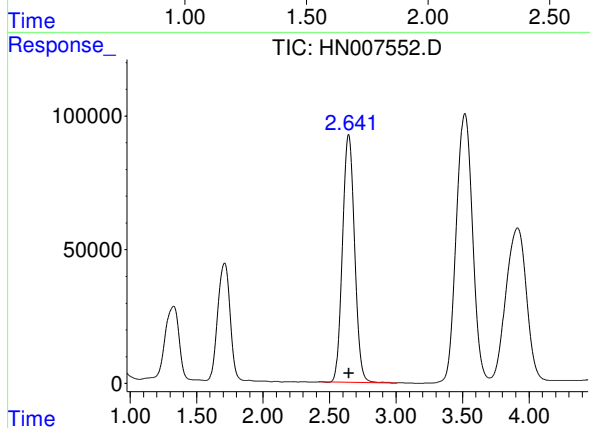

#4 1,3,5-Trinitrobenzene


R.T.: 2.643 min
Delta R.T.: 0.000 min
Response: 5883206
Conc: 500.00 ug/L

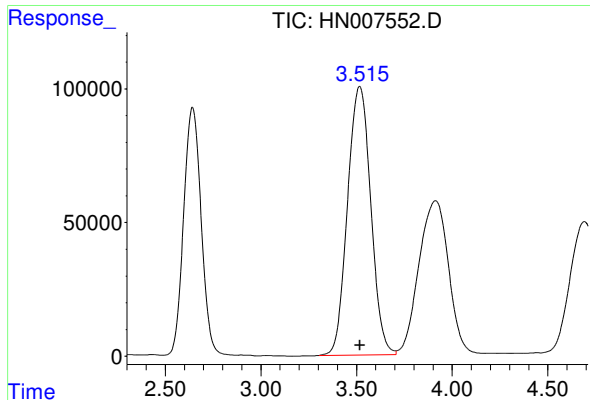

#5 1,3-Dinitrobenzene


R.T.: 3.517 min
Delta R.T.: 0.000 min
Response: 8493404
Conc: 500.00 ng/ml

Instrument :
HPLC_N
ClientSampleId :
SSTDICCC0500

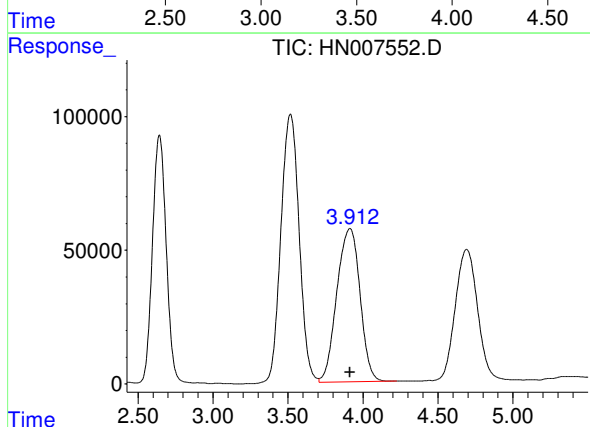


#6 3,5-Dinitroaniline

R.T.: 3.914 min
Delta R.T.: 0.000 min
Response: 6159773
Conc: 500.00 ug/L

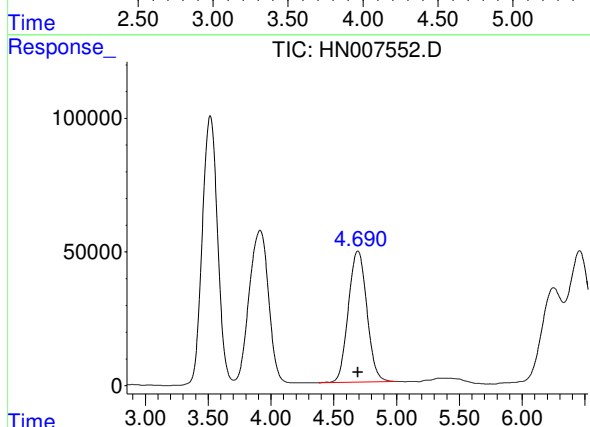


#7 Nitrobenzene

R.T.: 4.692 min
Delta R.T.: 0.000 min
Response: 5038872
Conc: 500.00 ug/L

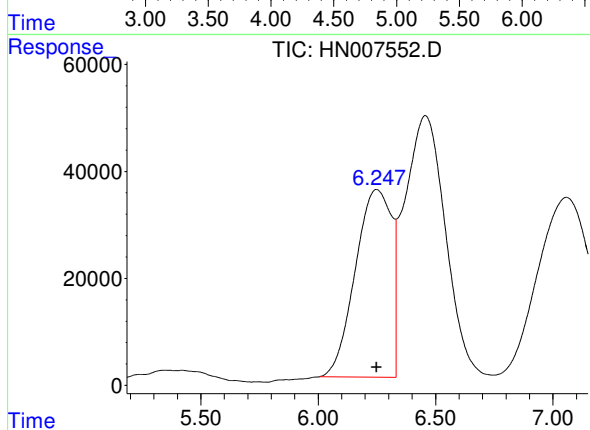

#8 Tetryl


R.T.: 6.249 min
Delta R.T.: 0.000 min
Response: 3774085
Conc: 500.00 ug/L

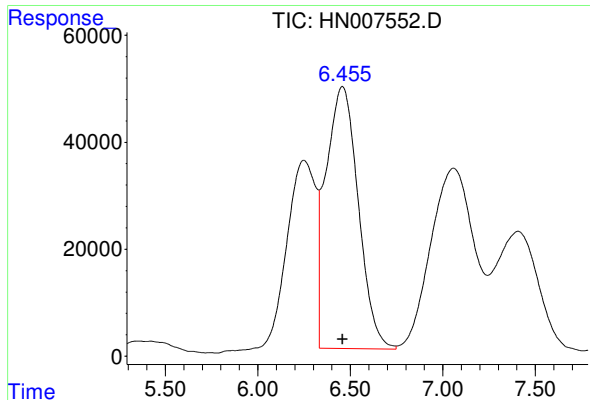

#9 2,4,6-Trinitrotoluene


R.T.: 6.457 min
Delta R.T.: 0.000 min
Response: 5958008
Conc: 500.00 ug/L

Instrument :
HPLC_N
ClientSampleId :
SSTDICCC0500

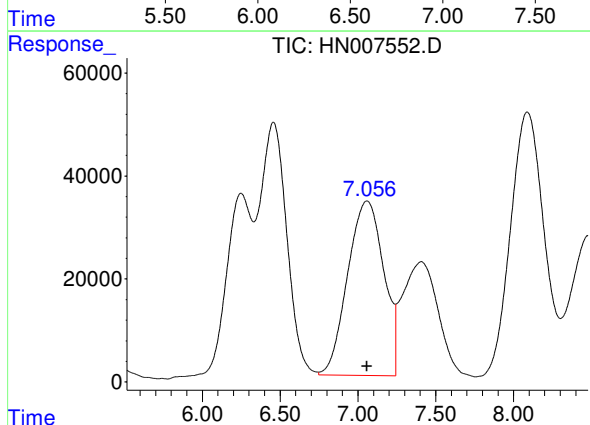


#10 2-Amino-4,6-dinitrotoluene

R.T.: 7.058 min
Delta R.T.: 0.000 min
Response: 5480711
Conc: 500.00 ug/L

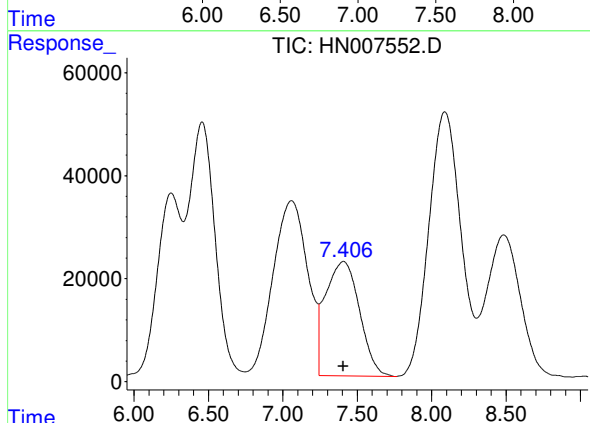


#11 4-Amino-2,6-dinitrotoluene

R.T.: 7.407 min
Delta R.T.: 0.000 min
Response: 3527012
Conc: 500.00 ug/L

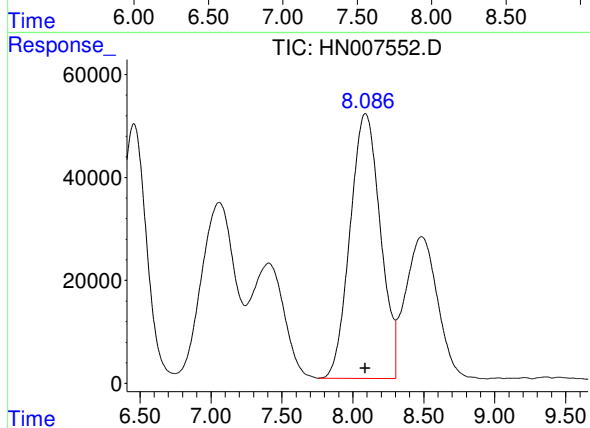

#12 2,4-Dinitrotoluene


R.T.: 8.089 min
Delta R.T.: 0.000 min
Response: 7650239
Conc: 500.00 ug/L

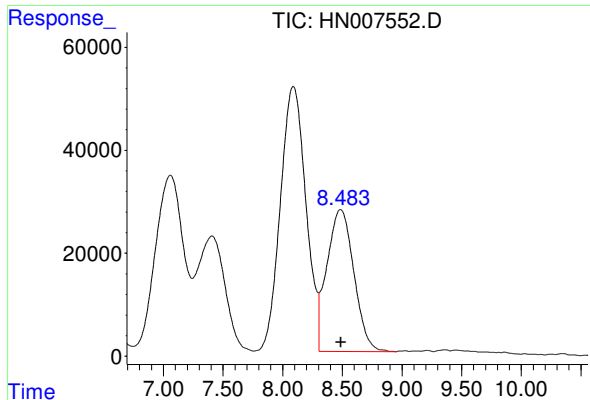

#13 2,6-Dinitrotoluene


R.T.: 8.485 min
Delta R.T.: 0.000 min
Response: 4348716
Conc: 500.00 ug/L

Instrument :
HPLC_N
ClientSampleId :
SSTDICCC0500

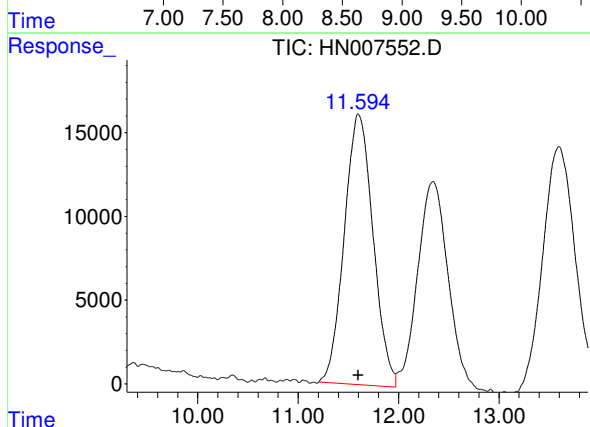


#14 2-Nitrotoluene

R.T.: 11.600 min
Delta R.T.: 0.000 min
Response: 3219116
Conc: 500.00 ug/L

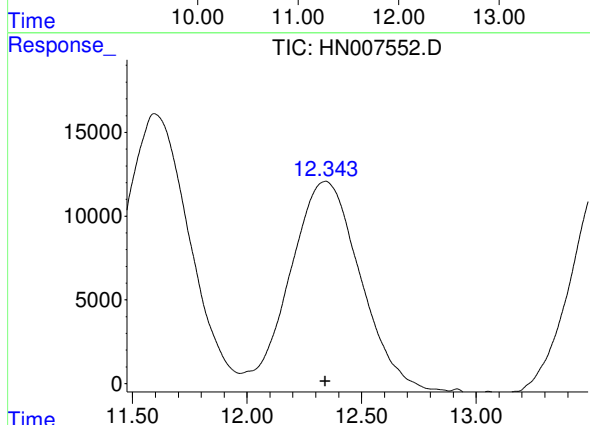


#15 4-Nitrotoluene

R.T.: 12.342 min
Delta R.T.: 0.000 min
Response: 2666014
Conc: 500.00 ug/L

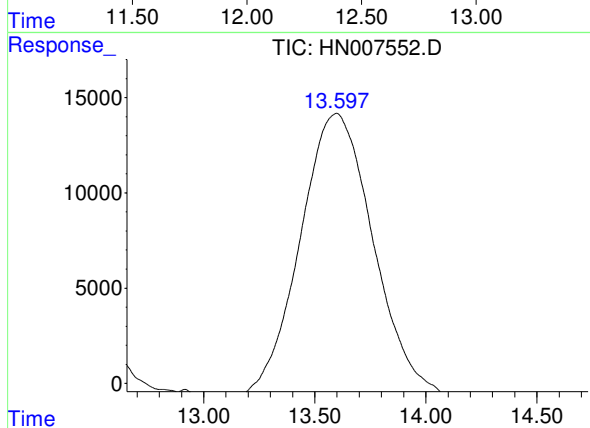

#16 3-Nitrotoluene

R.T.: 13.597 min
Delta R.T.: 0.000 min
Response: 3402565
Conc: 500.00 ug/L

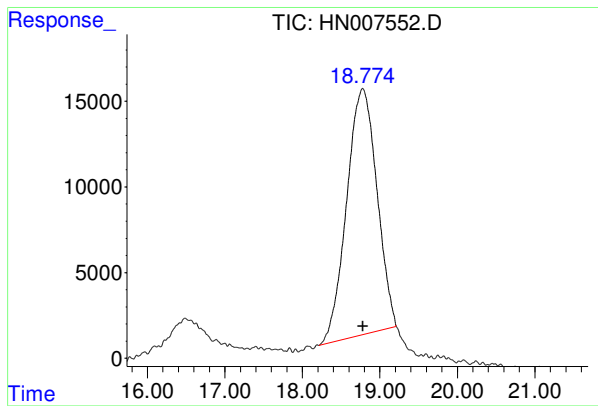

#17 PETN

R.T.: 18.777 min
Delta R.T.: 0.000 min
Response: 3896023
Conc: 500.00 ug/L

Instrument :
HPLC_N
ClientSampleId :
SSTDICCC0500