

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN100615\
Data File : HN007571.D
Signal(s) : vwd1A.ch
Acq On : 06-Oct-2015, 15:15
Operator : UM/MA
Sample : SSTDICC050
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
SSTDICC050

Integration File: AUTOINT1.E
Quant Time: Oct 06 17:19:50 2015
Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN1006NG.M
Quant Title :
QLast Update : Tue Oct 06 17:19:38 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.332	198763524	51.172 ng/ul
Target Compounds			
2) T Nitroglycerin	5.992	406248619	50.131 ng/ul

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN100615\
Data File : HN007571.D
Signal(s) : vwd1A.ch
Acq On : 06-Oct-2015, 15:15
Operator : UM/MA
Sample : SSTDICC050
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
SSTDICC050

Integration File: AUTOINT1.E
Quant Time: Oct 06 17:19:50 2015
Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN1006NG.M
Quant Title :
QLast Update : Tue Oct 06 17:19:38 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

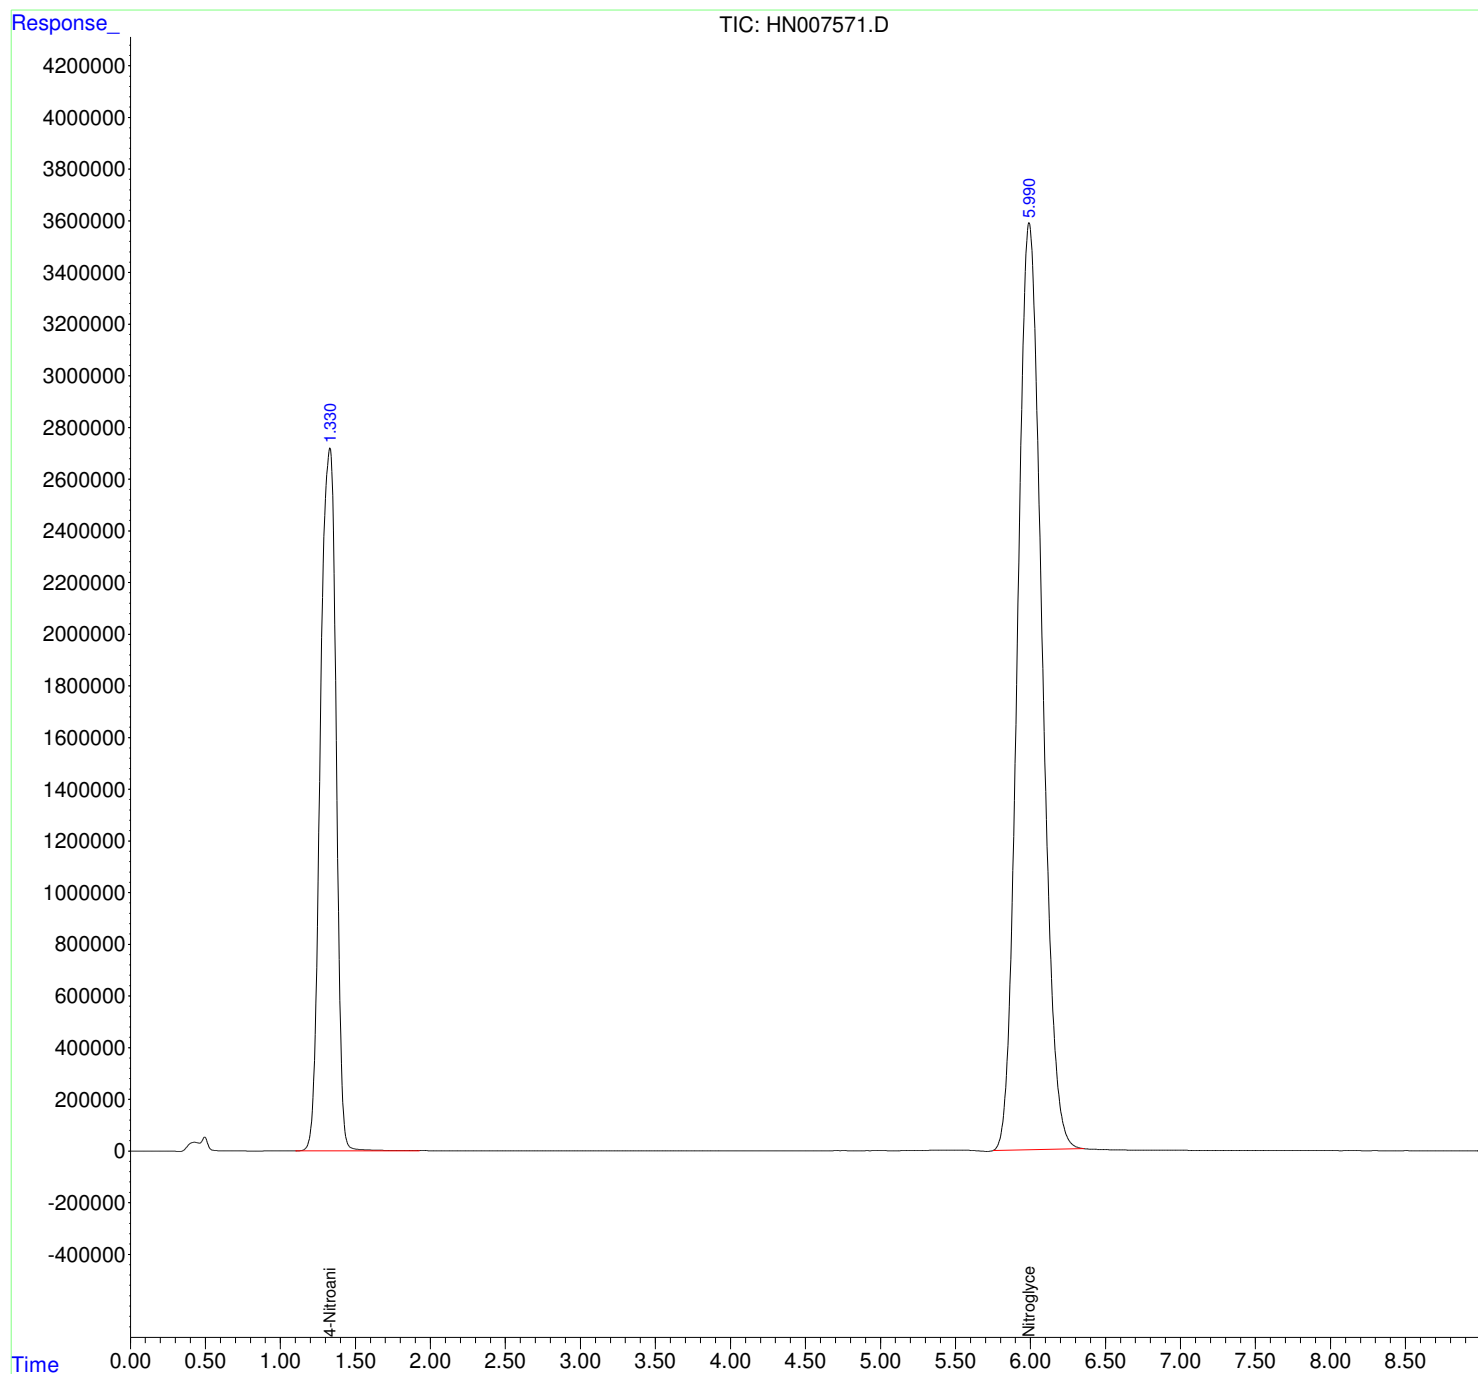


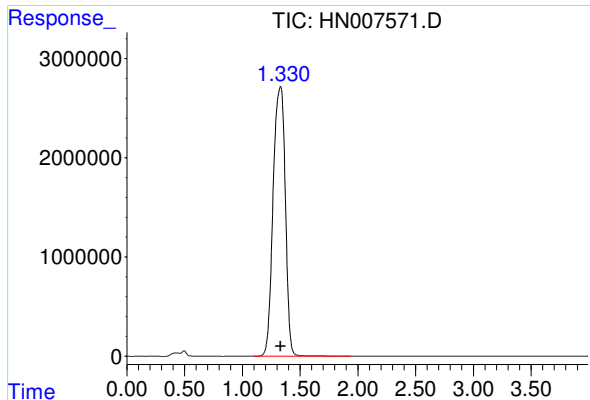

#1 4-Nitroaniline

R.T.: 1.332 min
Delta R.T.: 0.000 min
Response: 198763524
Conc: 51.17 ng/u1

Instrument :
HPLC_N
ClientSampleId :
SSTDIC050

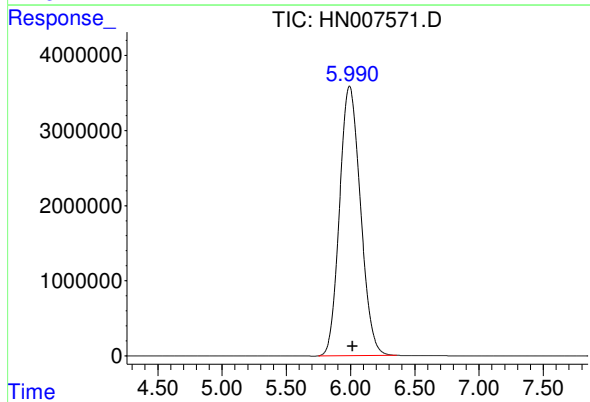

#2 Nitroglycerin

R.T.: 5.992 min
Delta R.T.: -0.023 min
Response: 406248619
Conc: 50.13 ng/u1